
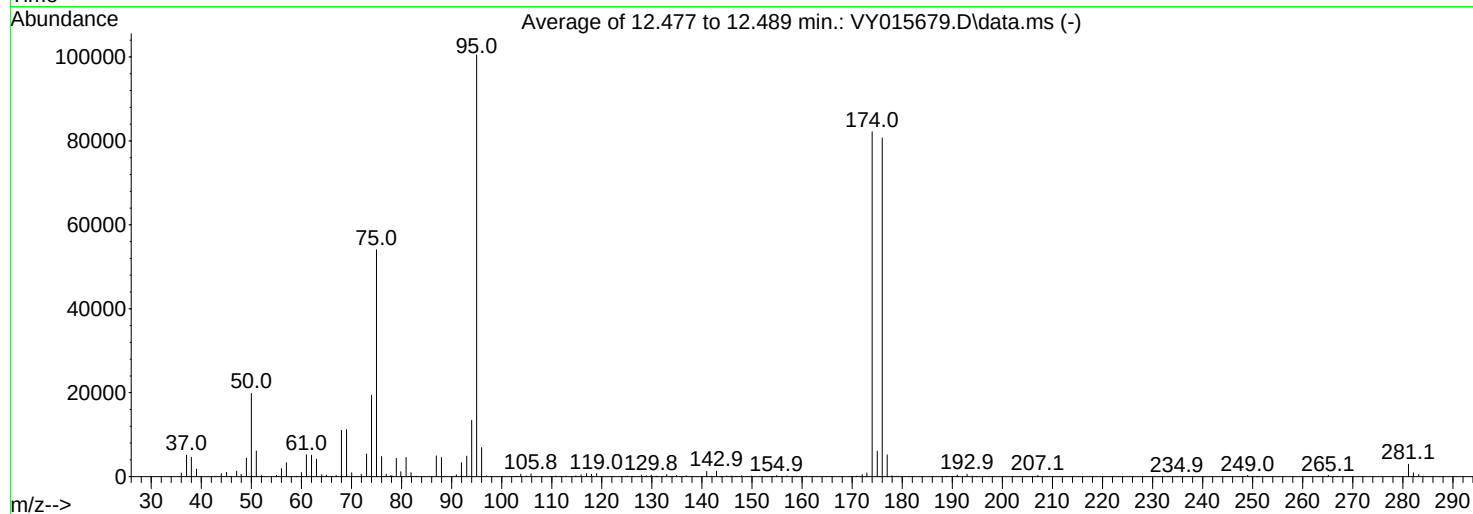


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092223\
Data File : VY015679.D
Acq On : 22 Sep 2023 11:37
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
Title : SW846 8260
Last Update : Wed Sep 20 01:39:40 2023

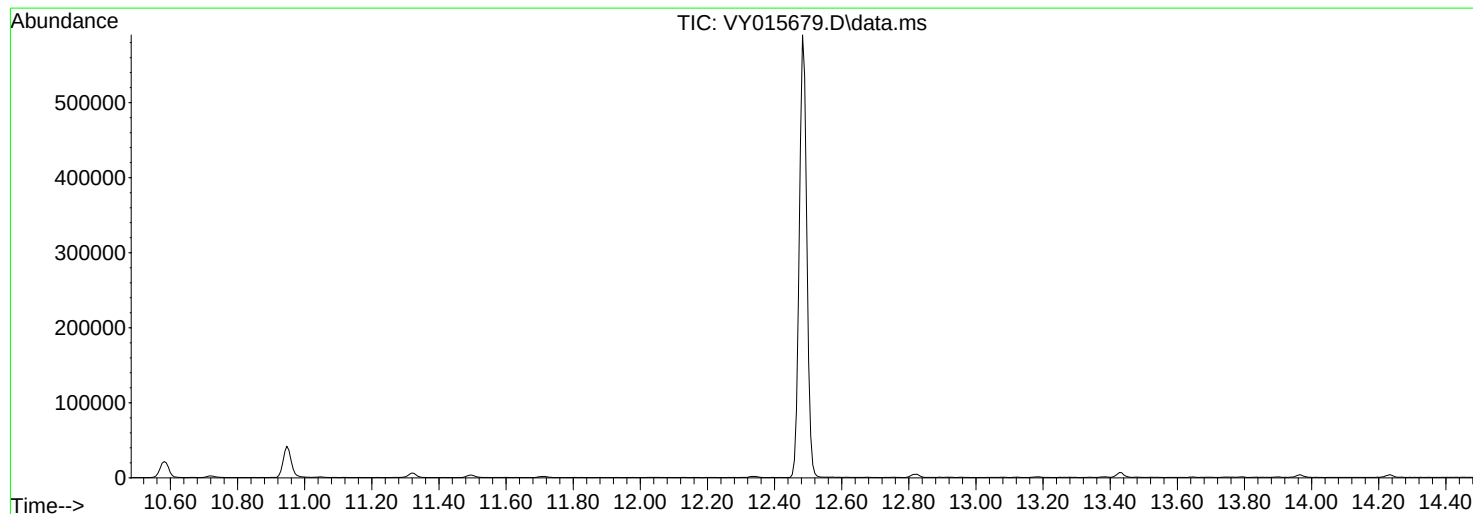

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	19843	PASS
75	95	30	60	53.8	54080	PASS
95	95	100	100	100.0	100515	PASS
96	95	5	9	6.9	6942	PASS
173	174	0.00	2	1.1	880	PASS
174	95	50	100	81.7	82157	PASS
175	174	5	9	7.4	6086	PASS
176	174	95	101	98.3	80723	PASS
177	176	5	9	6.4	5203	PASS