


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv092319\
 Data File : VY000124.D
 Acq On : 23 Sep 2019 10:04
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y092319S.M
 Title : SW846 8260
 Last Update : Tue Sep 24 05:14:45 2019

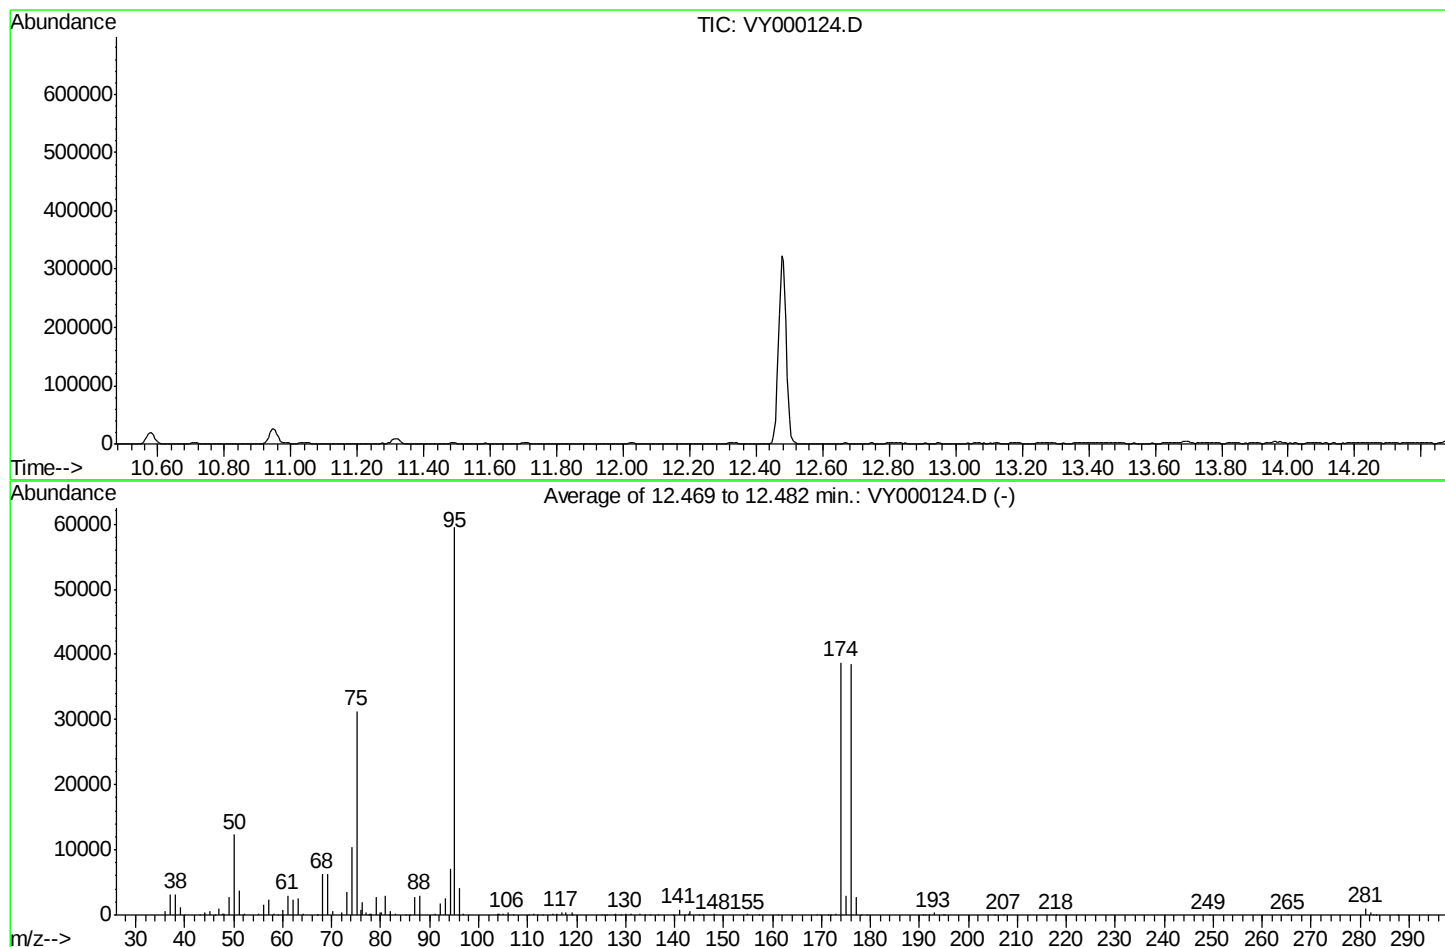

AutoFind: Scans 1785, 1786, 1787; Background Corrected with Scan 1778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	12292	PASS
75	95	30	60	52.5	31258	PASS
95	95	100	100	100.0	59504	PASS
96	95	5	9	7.1	4219	PASS
173	174	0.00	2	0.6	251	PASS
174	95	50	100	65.2	38794	PASS
175	174	5	9	7.7	3000	PASS
176	174	95	101	99.5	38602	PASS
177	176	5	9	6.9	2676	PASS