
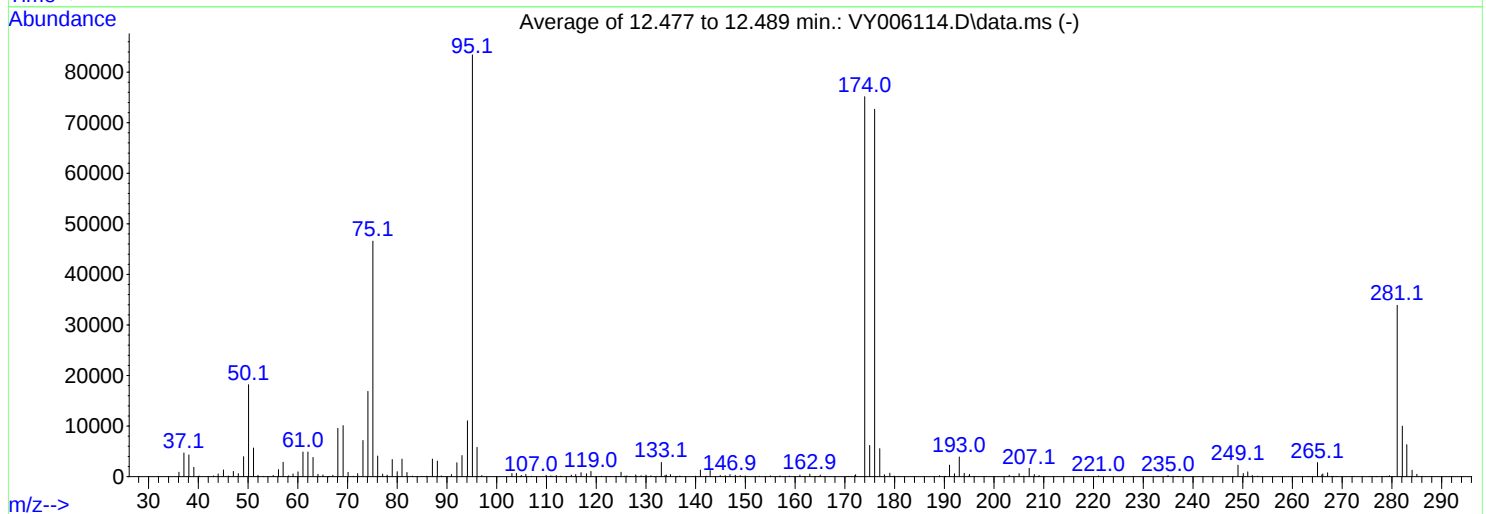


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092321\
Data File : VY006114.D
Acq On : 23 Sep 2021 09:09
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
Title : SW846 8260
Last Update : Wed Sep 15 05:01:47 2021

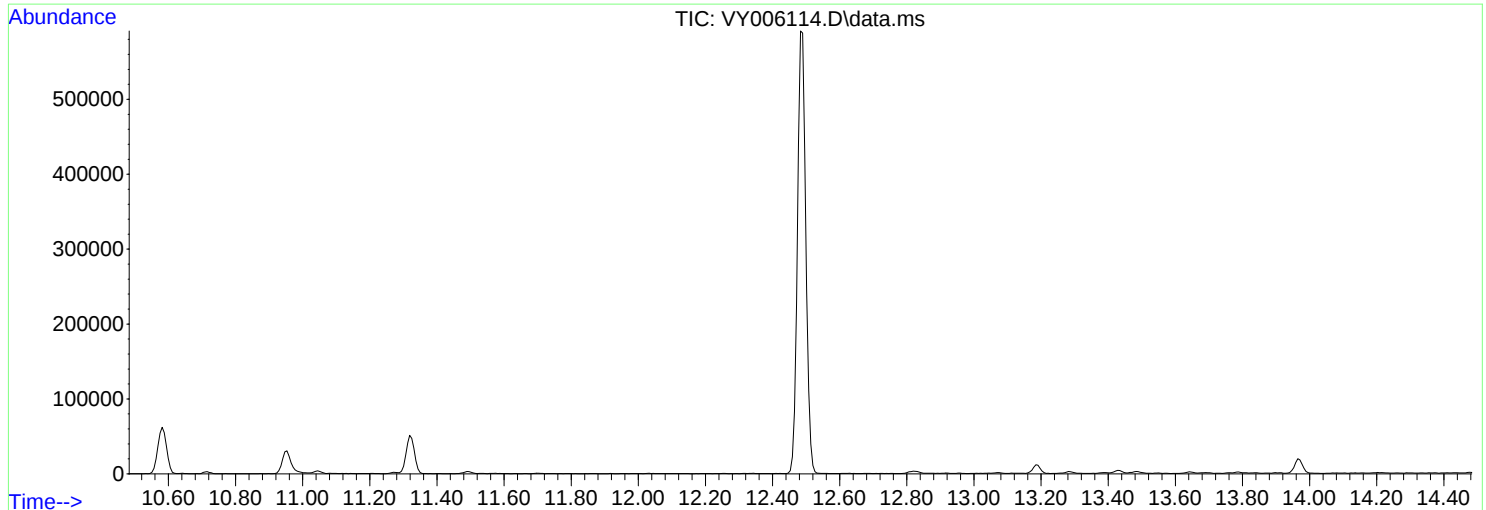

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	18205	PASS
75	95	30	60	55.8	46587	PASS
95	95	100	100	100.0	83421	PASS
96	95	5	9	6.9	5786	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.1	75144	PASS
175	174	5	9	8.2	6166	PASS
176	174	95	101	96.7	72651	PASS
177	176	5	9	7.6	5554	PASS