



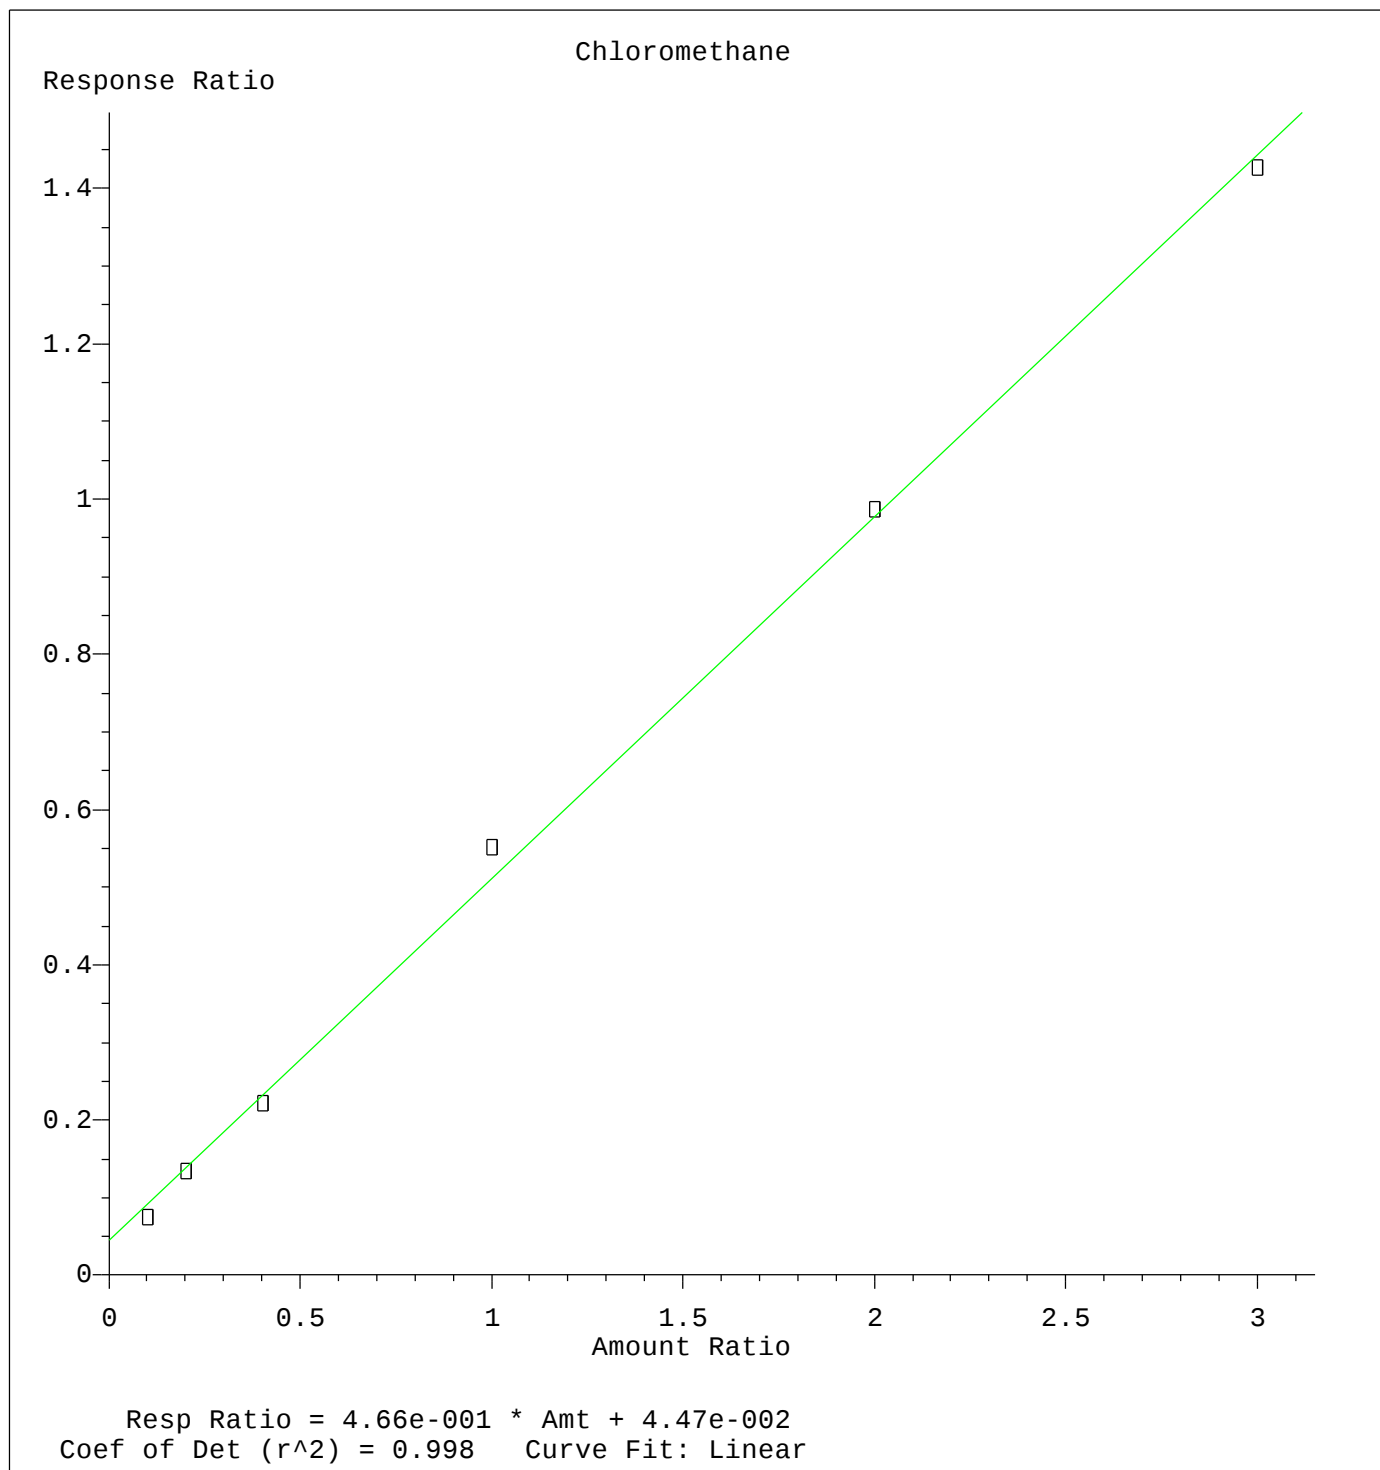


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y092619S.M
Calibration Table Last Updated: Thu Sep 26 14:30:12 2019

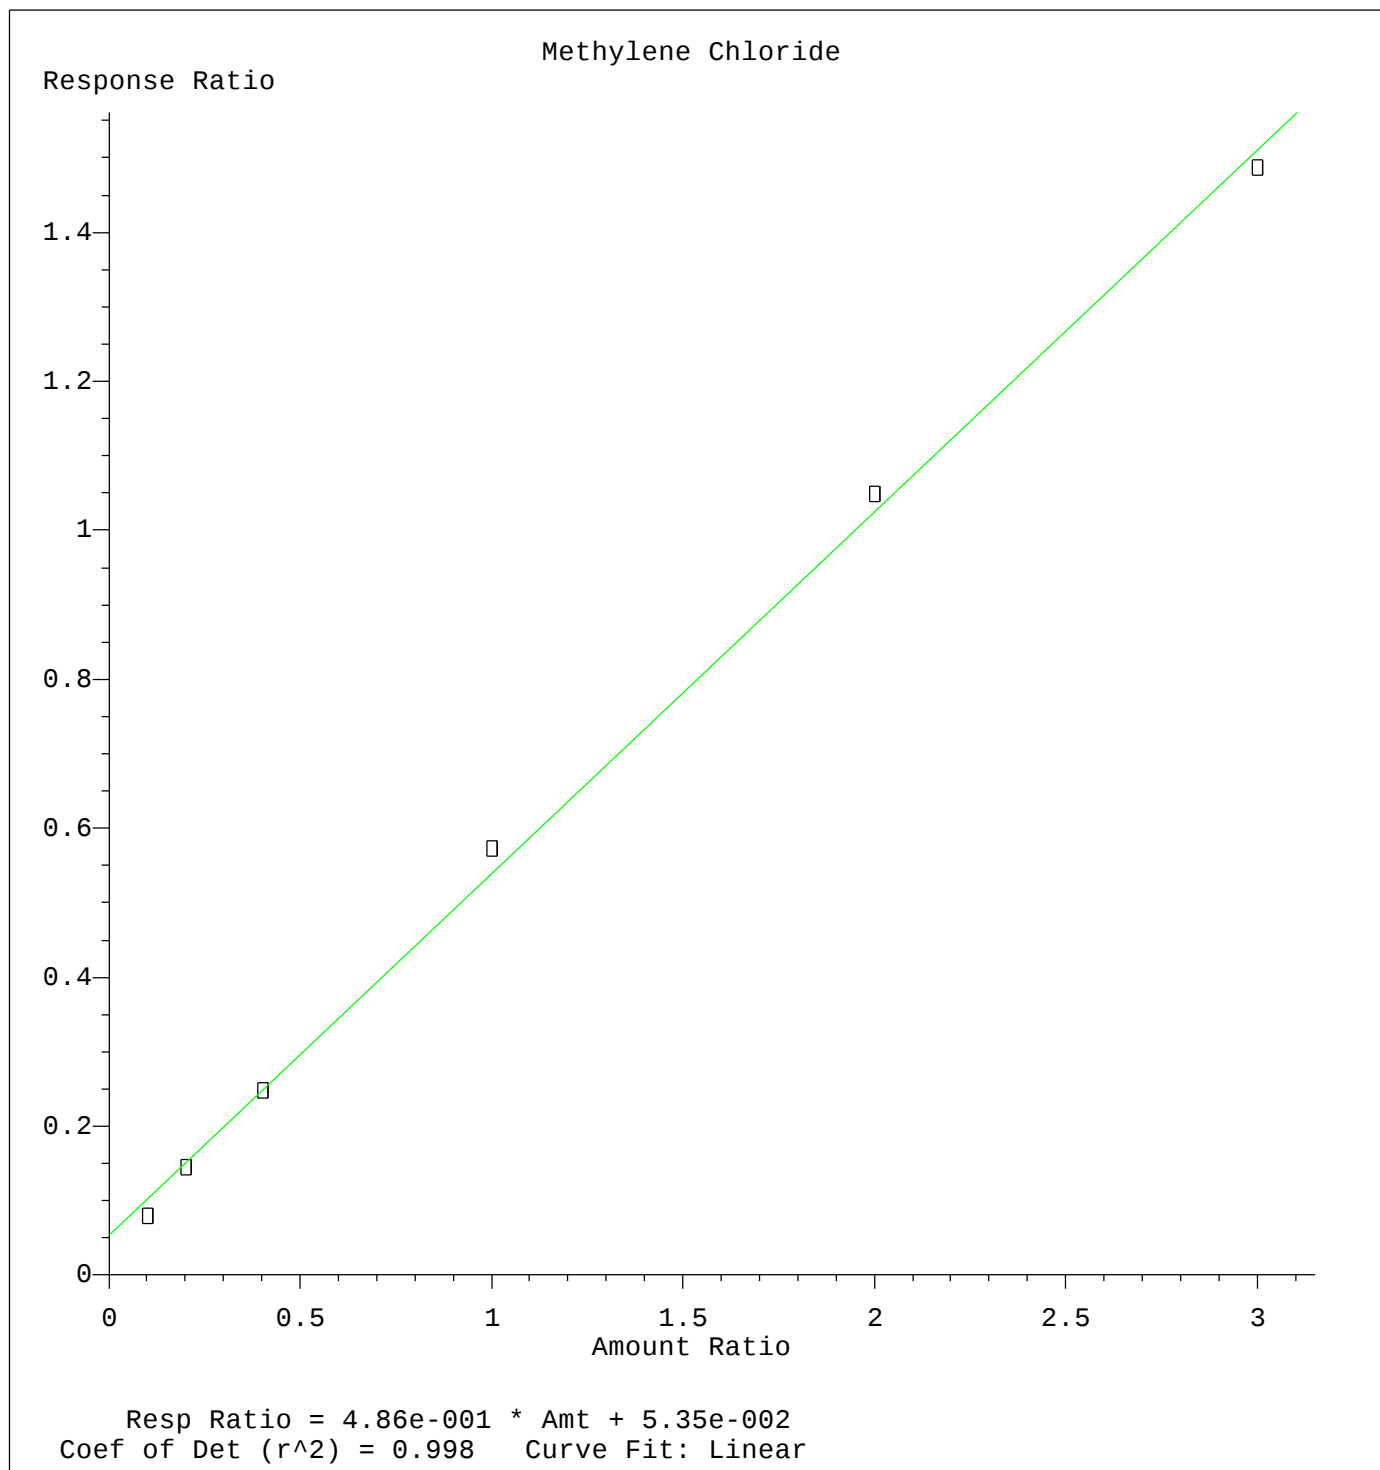

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y092619S.M
Calibration Table Last Updated: Thu Sep 26 14:30:12 2019

Dichlorodifluoromethane

Response Ratio

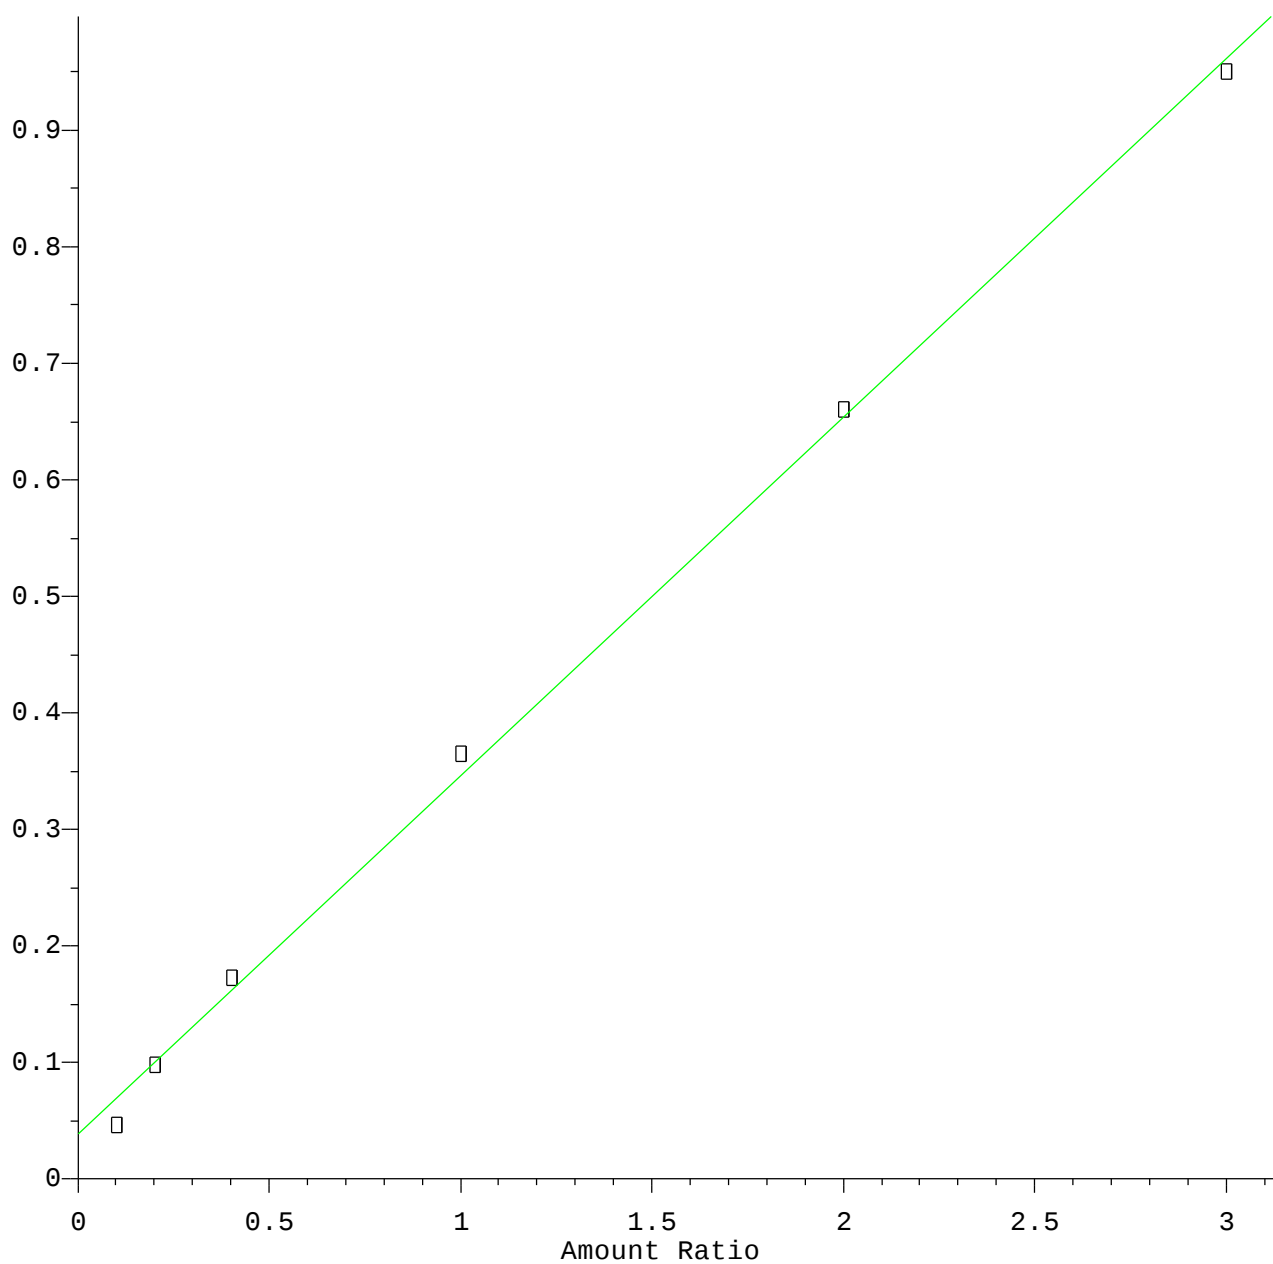

Resp Ratio = $3.08 \times 10^{-1} \times \text{Amt} + 3.79 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y092619S.M
Calibration Table Last Updated: Thu Sep 26 14:30:12 2019