


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv092619\
Data File : VY000141.D
Acq On : 26 Sep 2019 09:28
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y092619S.M
Title : SW846 8260
Last Update : Thu Sep 26 14:30:12 2019

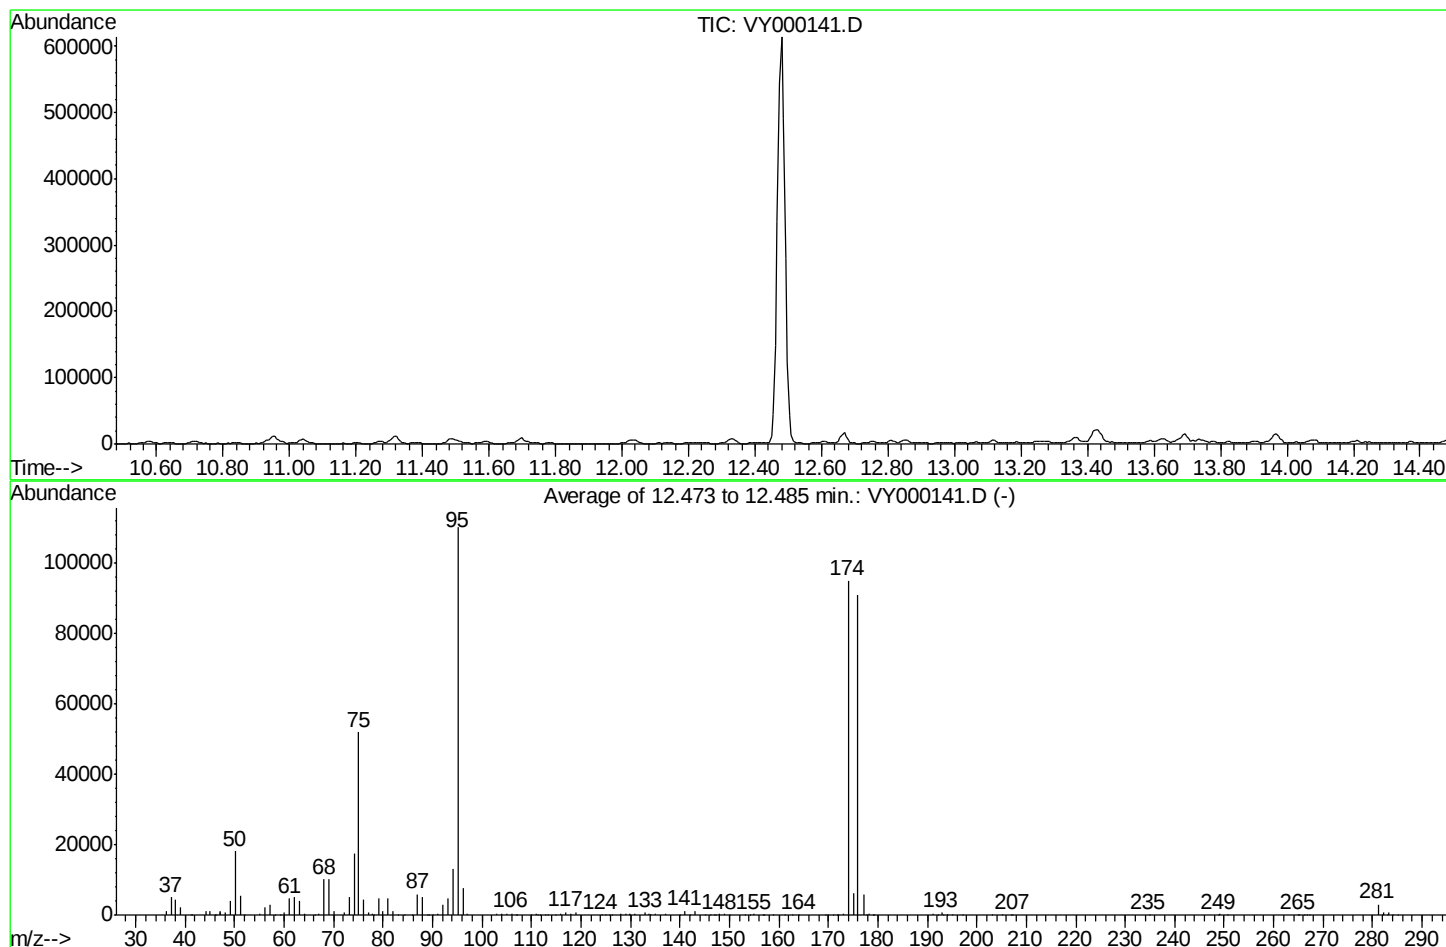

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	18039	PASS
75	95	30	60	47.2	51960	PASS
95	95	100	100	100.0	110120	PASS
96	95	5	9	6.9	7643	PASS
173	174	0.00	2	0.6	556	PASS
174	95	50	100	86.2	94968	PASS
175	174	5	9	6.4	6039	PASS
176	174	95	101	95.8	90949	PASS
177	176	5	9	6.6	6011	PASS