
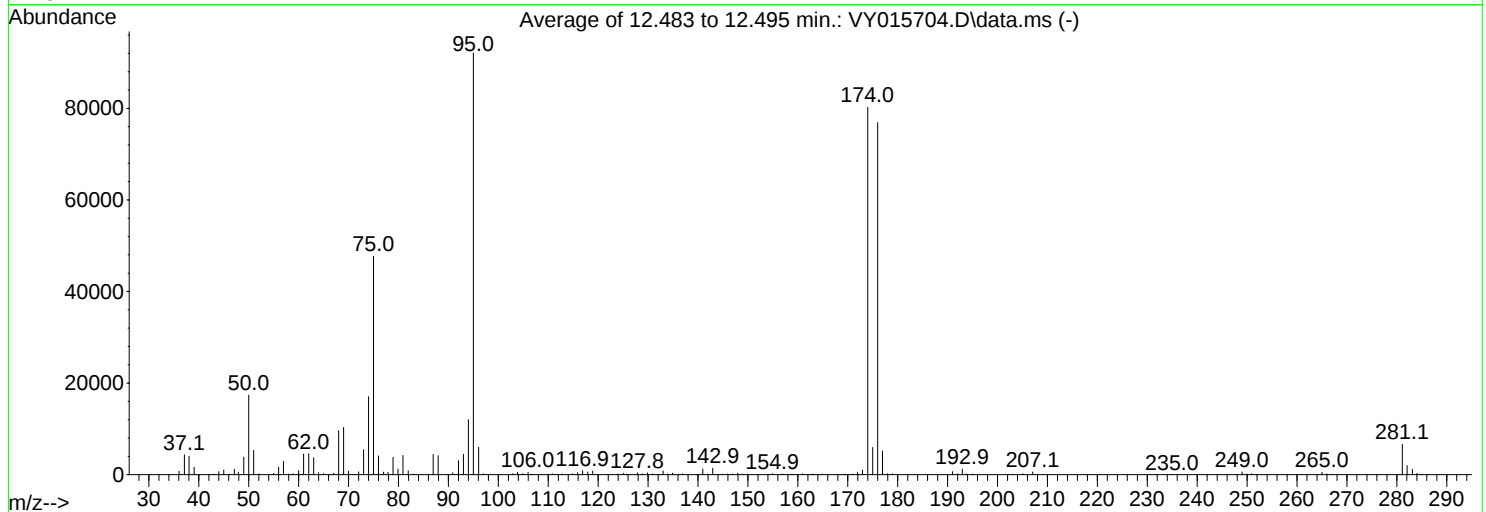


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092623\
Data File : VY015704.D
Acq On : 26 Sep 2023 08:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
Title : SW846 8260
Last Update : Wed Sep 20 01:39:40 2023

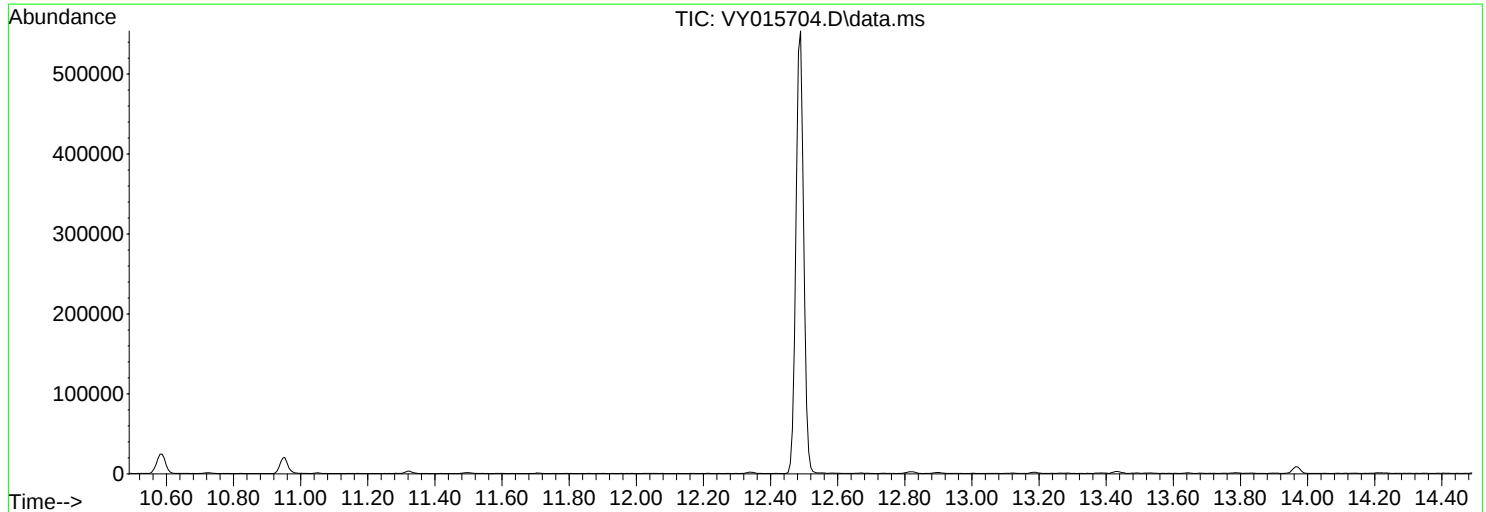

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	17363	PASS
75	95	30	60	51.8	47688	PASS
95	95	100	100	100.0	92115	PASS
96	95	5	9	6.5	5981	PASS
173	174	0.00	2	1.2	968	PASS
174	95	50	100	87.1	80240	PASS
175	174	5	9	7.4	5927	PASS
176	174	95	101	95.9	76912	PASS
177	176	5	9	6.7	5171	PASS