


Methylene Chloride

Response Ratio

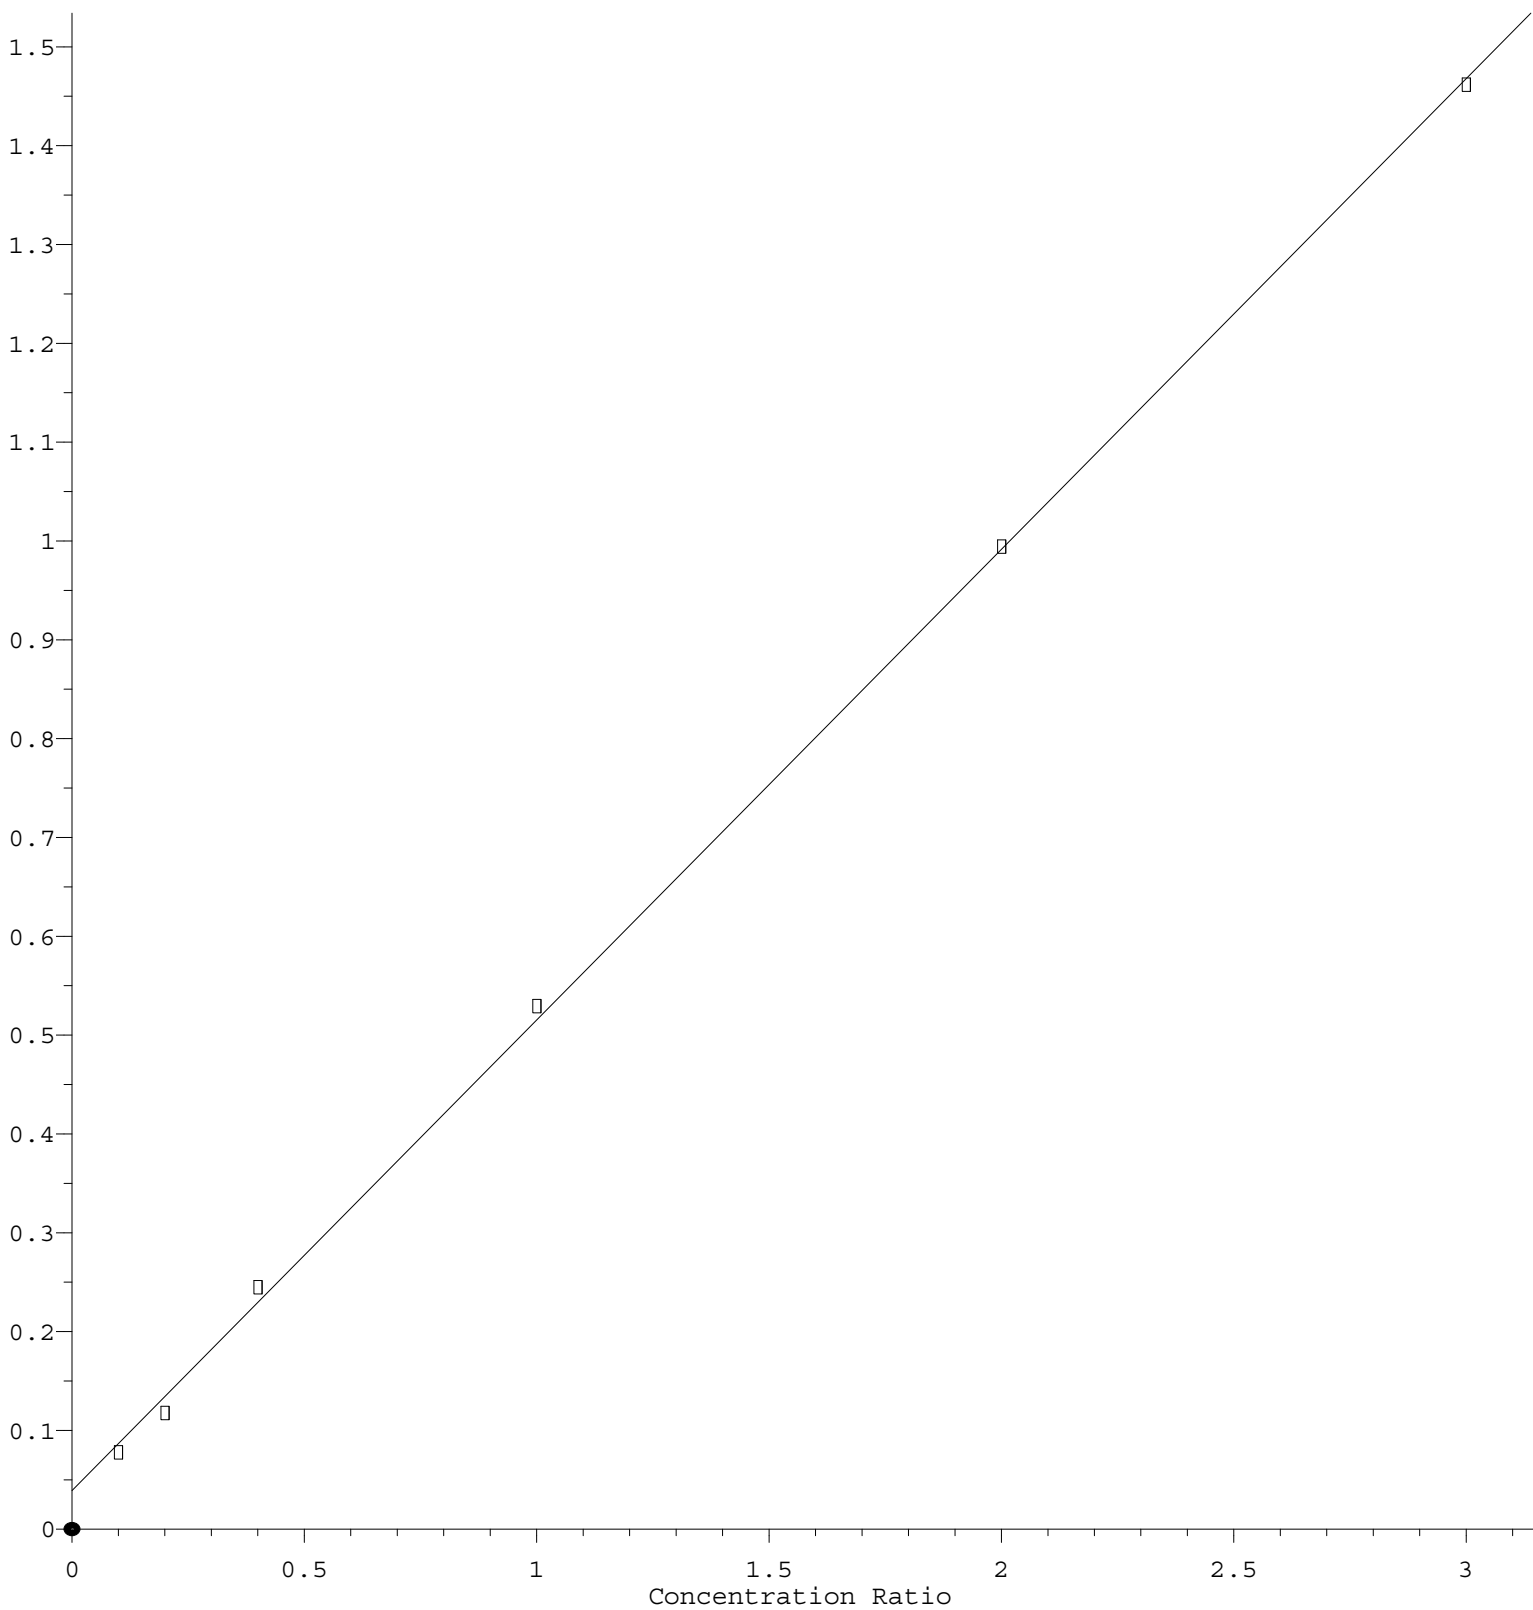


$$\text{Response} = 4.767\text{e-}001 * \text{Amt} + 3.858\text{e-}002$$

Coef of Det (r^2) = 0.999458 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y092821S.M

Calibration Table Last Updated: Tue Sep 28 17:44:36 2021

Acrolein

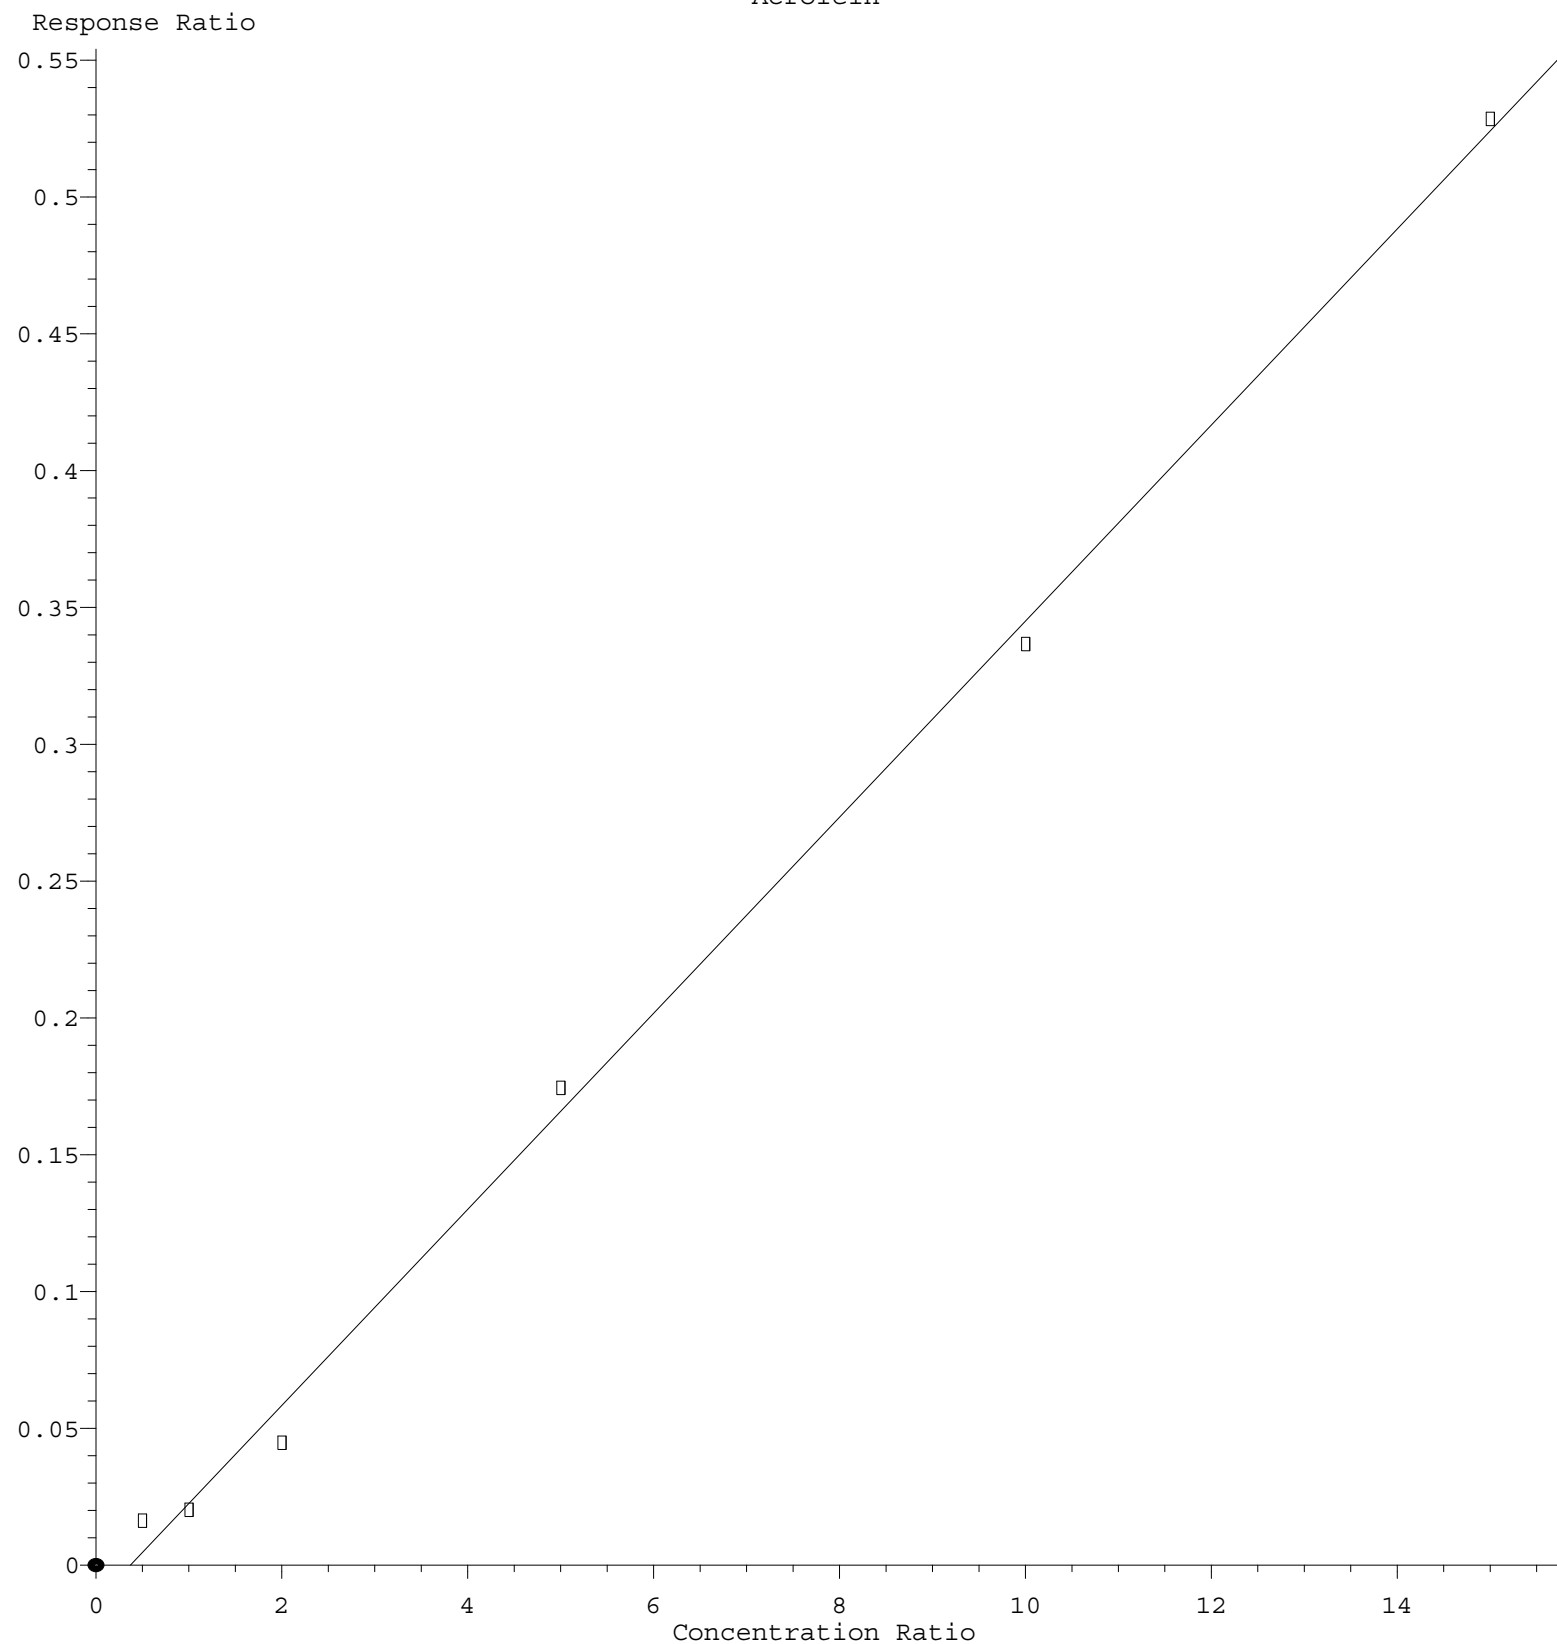

Response = $3.583 \times 10^{-2} \times \text{Amt} - 1.324 \times 10^{-2}$
 Coef of Det (r^2) = 0.997740 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y092821S.M
 Calibration Table Last Updated: Tue Sep 28 17:44:36 2021