
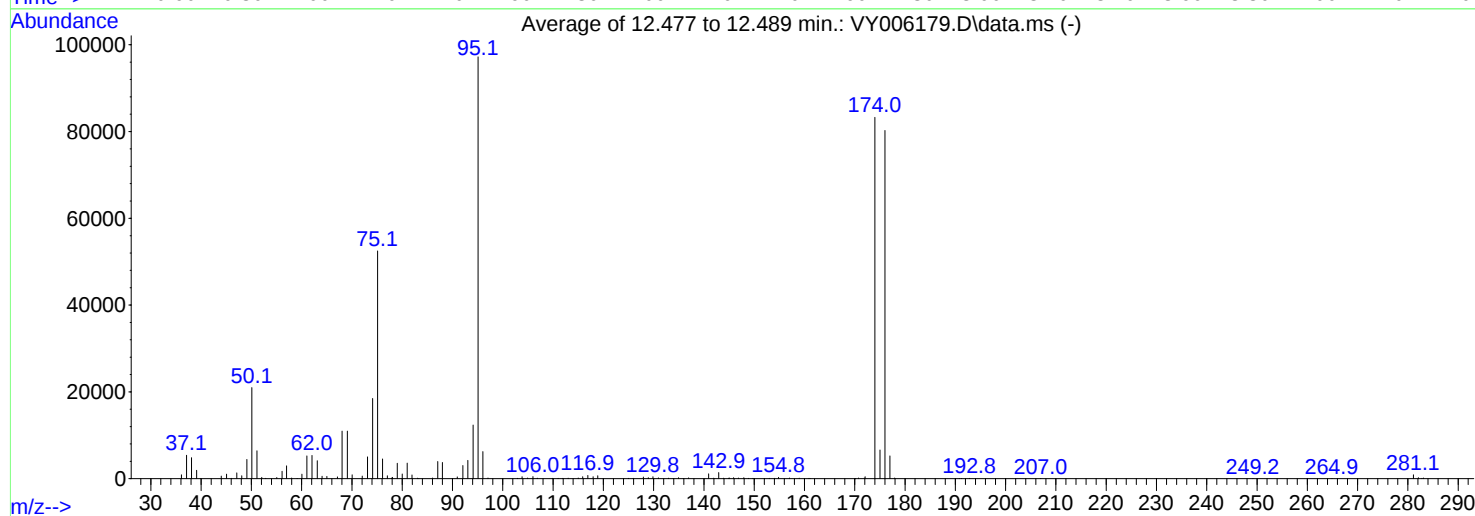


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092821\
 Data File : VY006179.D
 Acq On : 28 Sep 2021 09:07
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
 Title : SW846 8260
 Last Update : Tue Sep 28 17:44:36 2021

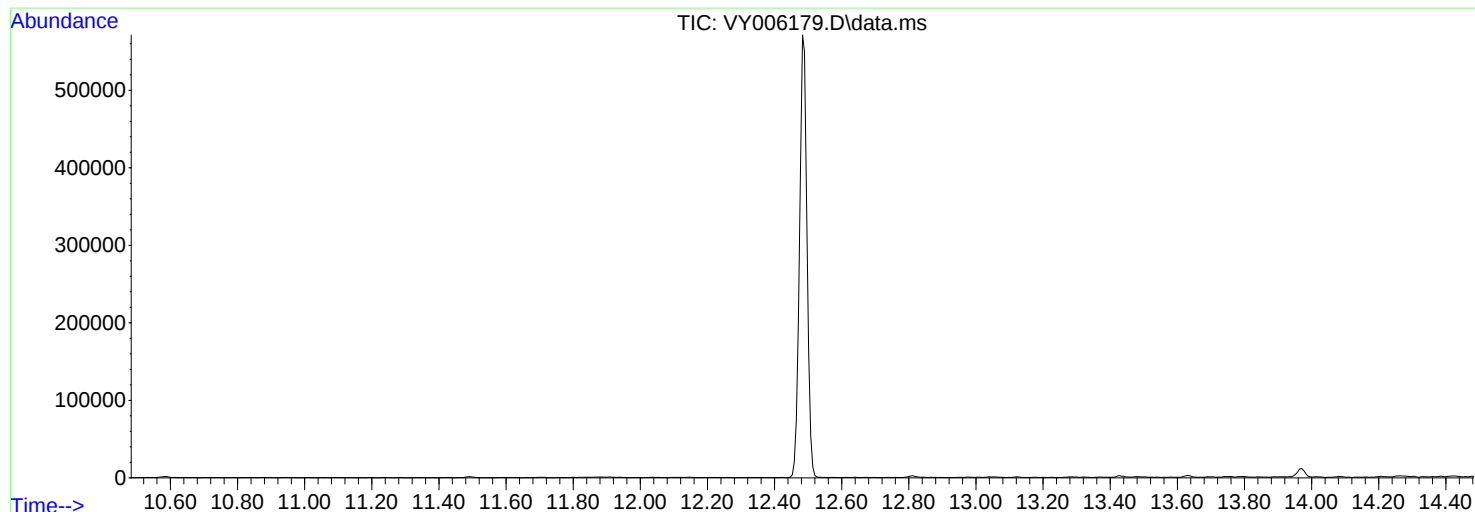

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	20981	PASS
75	95	30	60	54.0	52483	PASS
95	95	100	100	100.0	97221	PASS
96	95	5	9	6.4	6252	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.7	83285	PASS
175	174	5	9	7.9	6606	PASS
176	174	95	101	96.4	80256	PASS
177	176	5	9	6.5	5222	PASS