
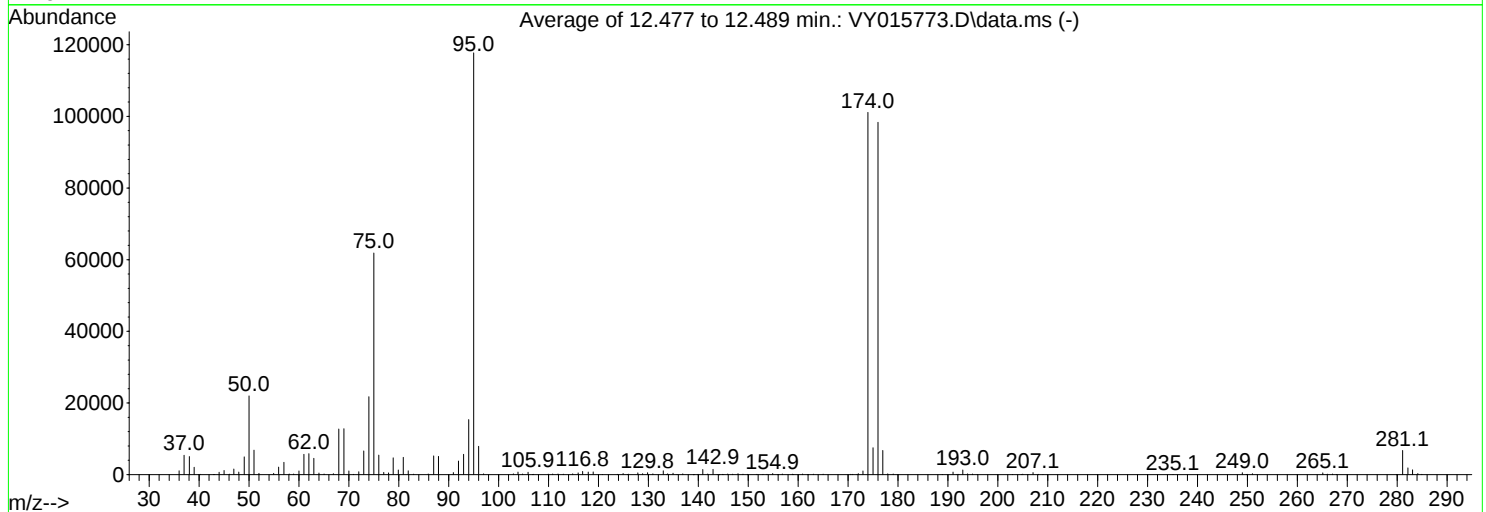


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100223\
Data File : VY015773.D
Acq On : 02 Oct 2023 10:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
Title : SW846 8260
Last Update : Wed Sep 20 01:39:40 2023

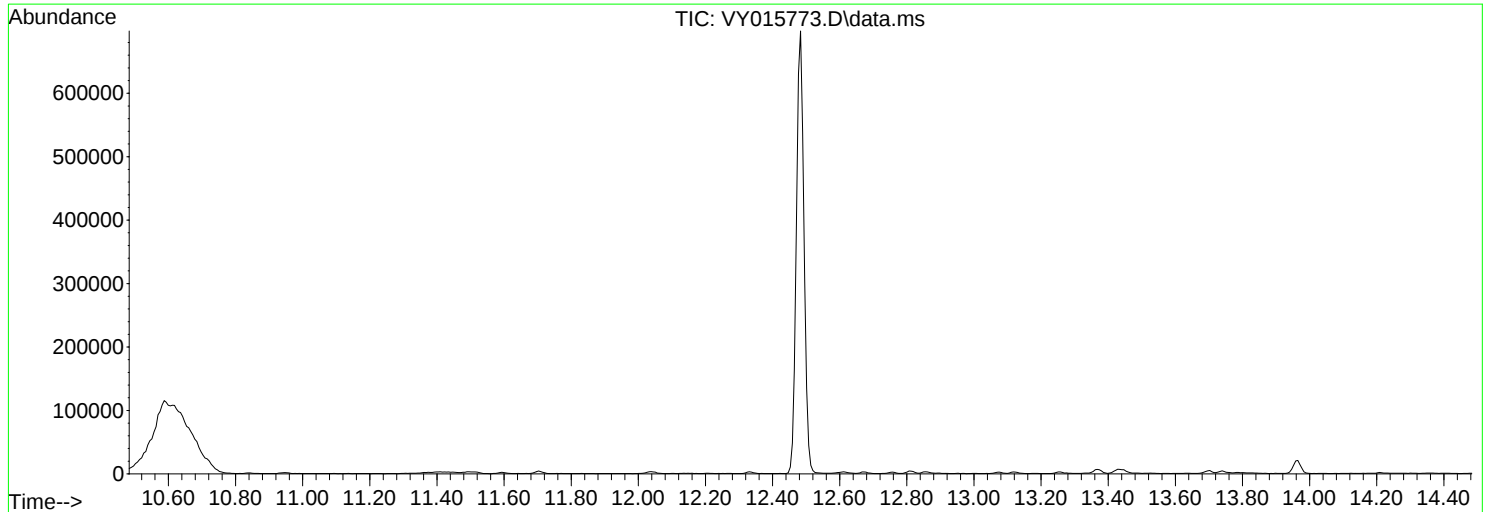

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	21955	PASS
75	95	30	60	52.5	61861	PASS
95	95	100	100	100.0	117736	PASS
96	95	5	9	6.7	7920	PASS
173	174	0.00	2	1.0	1010	PASS
174	95	50	100	85.9	101101	PASS
175	174	5	9	7.4	7485	PASS
176	174	95	101	97.3	98349	PASS
177	176	5	9	6.9	6739	PASS