


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY100319\
Data File : VY000181.D
Acq On : 03 Oct 2019 12:00
Operator : SY/MD
Sample : BFB
Misc : 5.0ml/MSVOA Y/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y100319W.M
Title : SW846 8260
Last Update : Fri Oct 04 06:00:29 2019

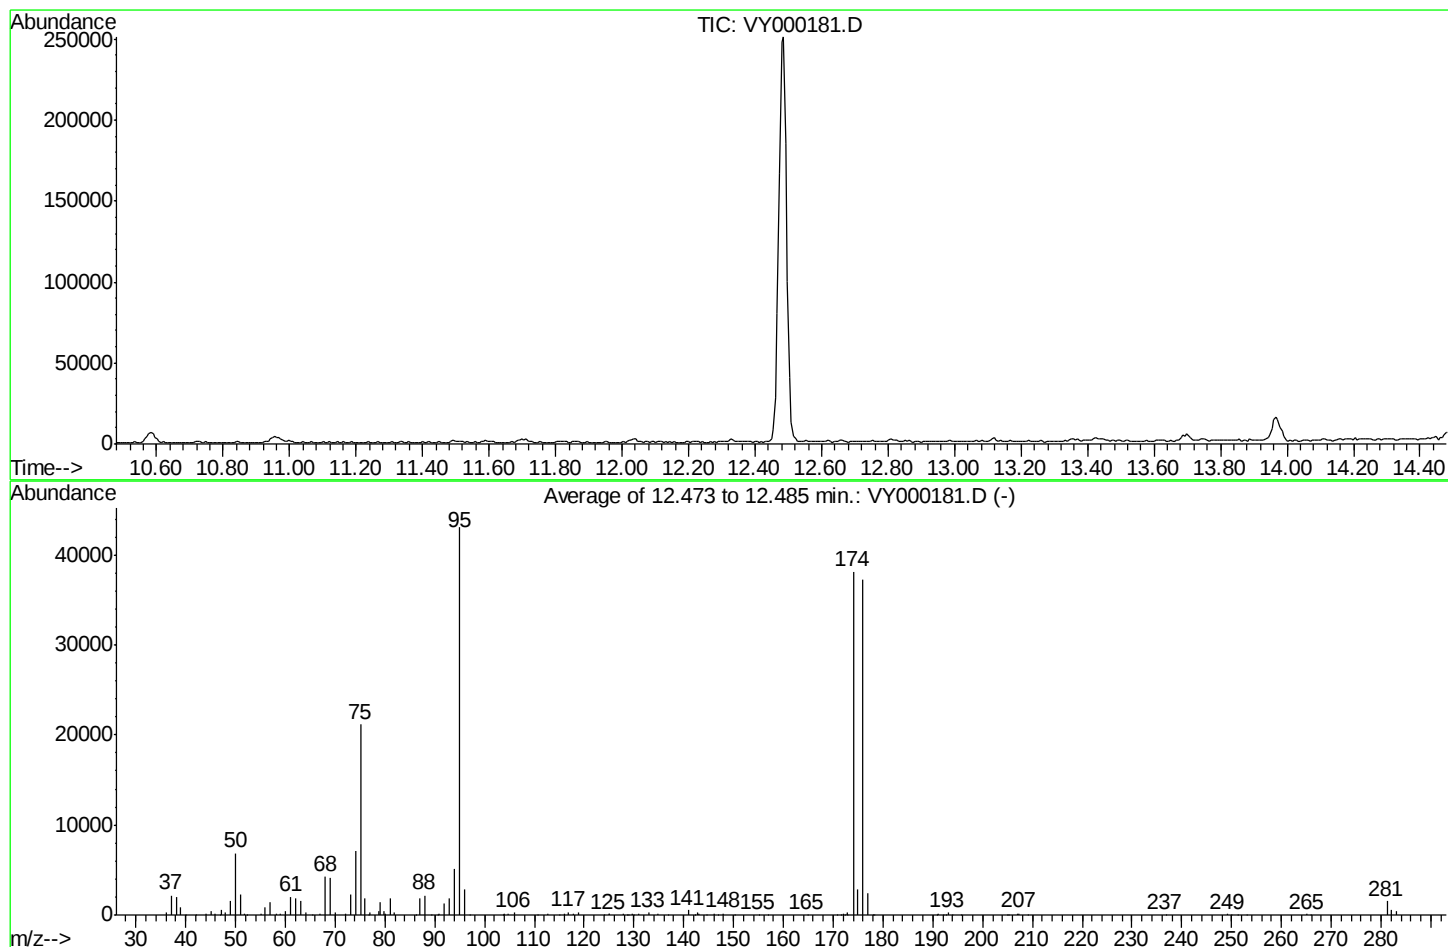

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	6846	PASS
75	95	30	60	49.2	21168	PASS
95	95	100	100	100.0	43058	PASS
96	95	5	9	6.6	2829	PASS
173	174	0.00	2	0.6	222	PASS
174	95	50	100	88.6	38138	PASS
175	174	5	9	7.4	2815	PASS
176	174	95	101	97.9	37325	PASS
177	176	5	9	6.6	2466	PASS