

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100421\
 Data File : VY006274.D
 Acq On : 04 Oct 2021 14:22
 Operator : SY/MD
 Sample : VY1004SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1004SBL01

Quant Time: Oct 05 06:36:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 28 17:44:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.837	168	108696	50.000	ug/l	0.04
34) 1,4-Difluorobenzene	8.721	114	172296	50.000	ug/l	0.02
63) Chlorobenzene-d5	11.501	117	154158	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	79699	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.179	65	61282	52.677	ug/l	0.03
Spiked Amount 50.000	Range 50 - 163		Recovery = 105.360%			
35) Dibromofluoromethane	7.758	113	44146	47.958	ug/l	0.04
Spiked Amount 50.000	Range 54 - 147		Recovery = 95.920%			
50) Toluene-d8	10.197	98	175036	45.434	ug/l	0.01
Spiked Amount 50.000	Range 49 - 140		Recovery = 90.860%			
62) 4-Bromofluorobenzene	12.483	95	58442	44.655	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 89.300%			
Target Compounds						
16) Acetone	4.058	43	342	1.053	ug/l #	47
31) Cyclohexane	7.837	56	2662	1.208	ug/l #	32
36) 1,1-Dichloropropene	7.837	75	8403	4.902	ug/l #	52
38) Carbon Tetrachloride	7.837	117	10652	5.885	ug/l #	15
76) 1,2,3-Trichloropropane	12.483	75	34229	44.187	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.483	75	34229	86.834	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100421\
Data File : VY006274.D
Acq On : 04 Oct 2021 14:22
Operator : SY/MD
Sample : VY1004SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01

Quant Time: Oct 05 06:36:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 17:44:36 2021
Response via : Initial Calibration




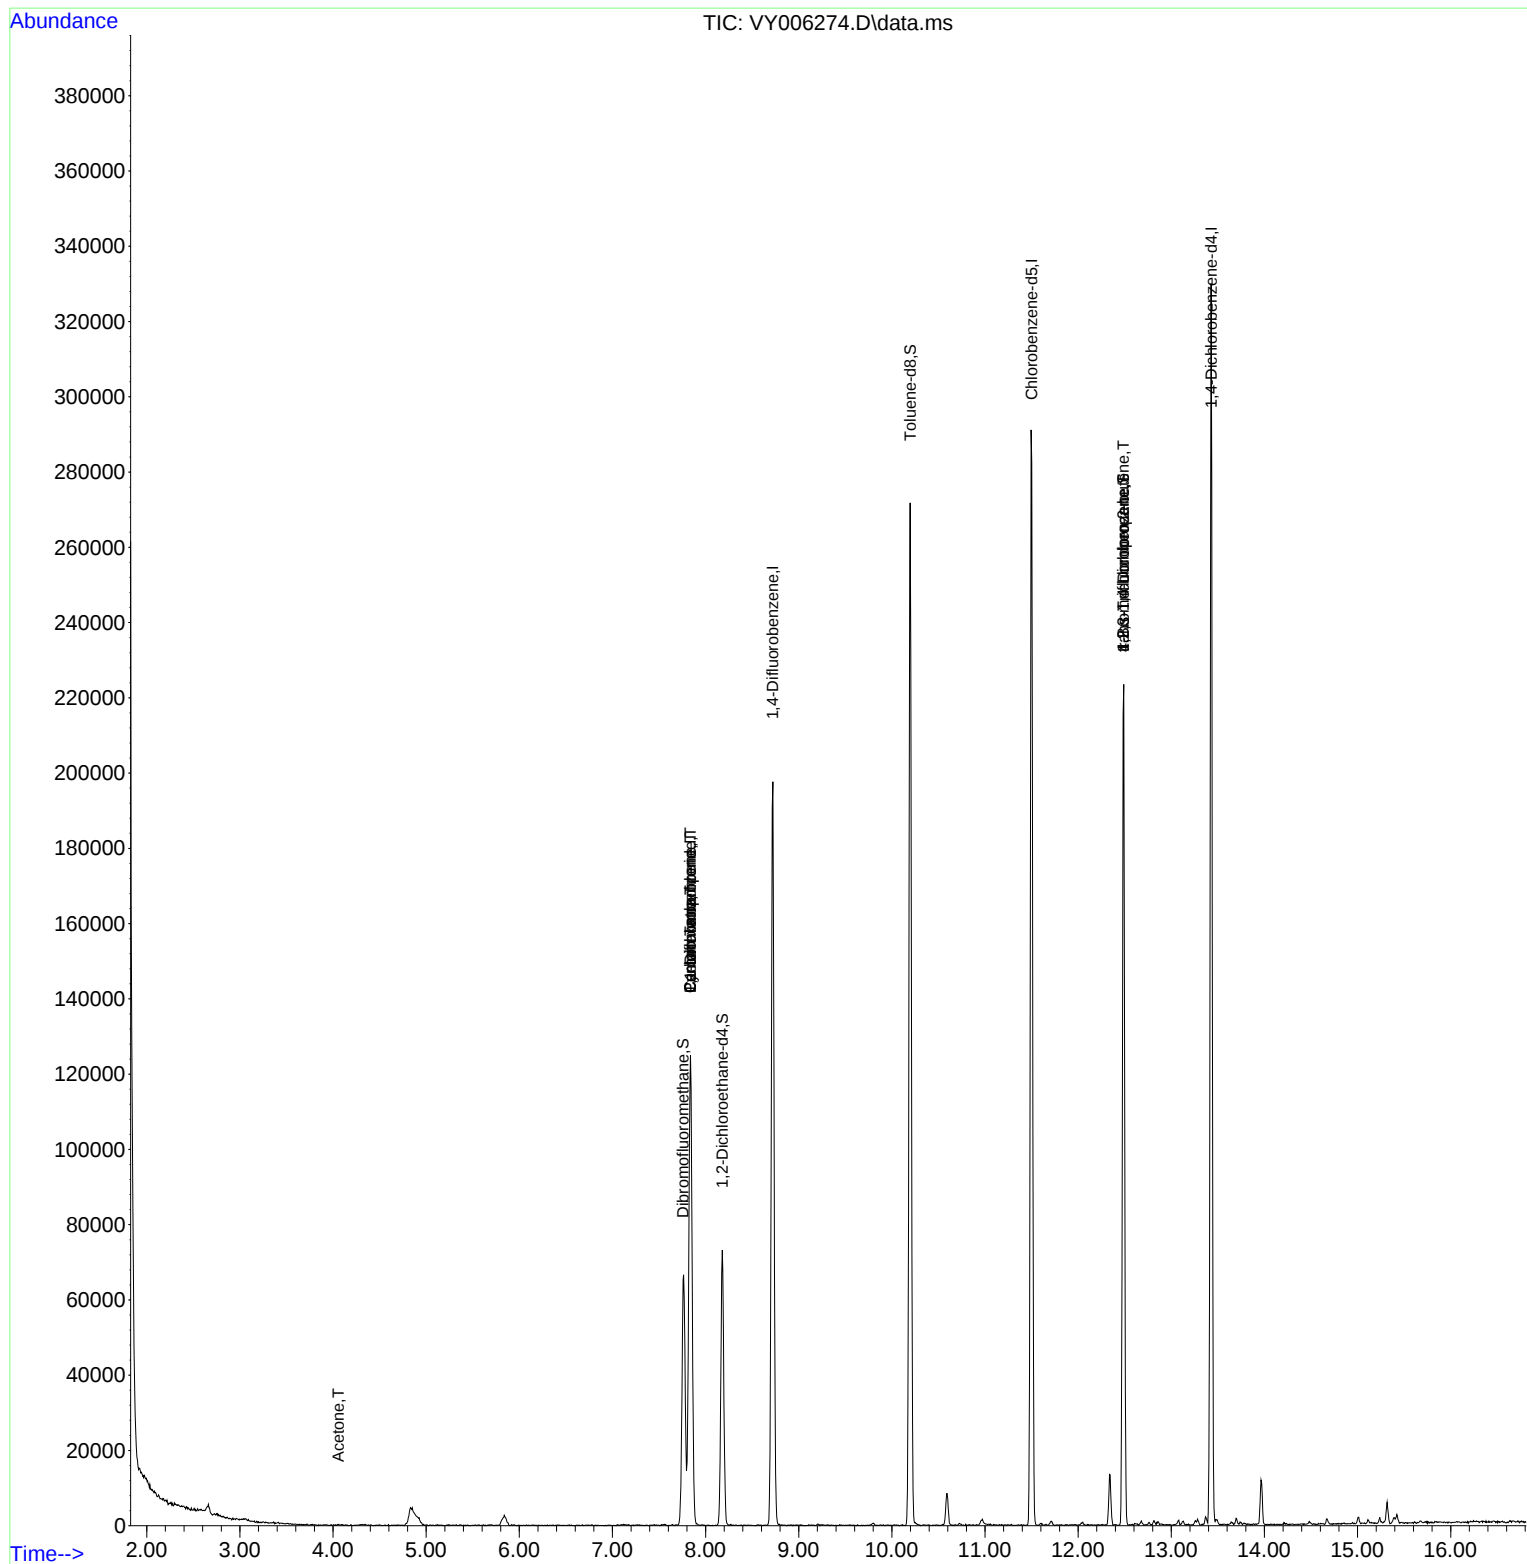


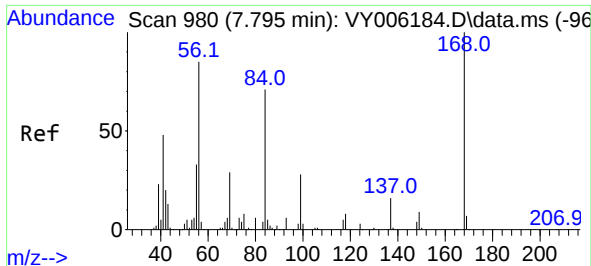

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.837 min Scan# 987
Delta R.T. 0.042 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22




Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01


Tgt Ion:168 Resp: 108696
Ion Ratio Lower Upper
168 100
99 54.3 46.9 70.3

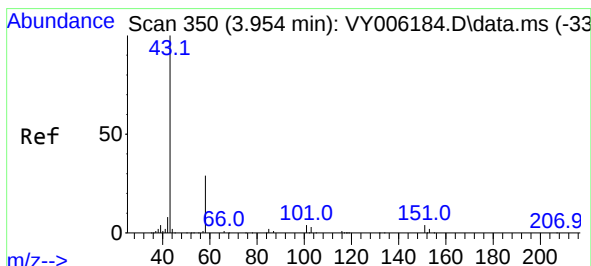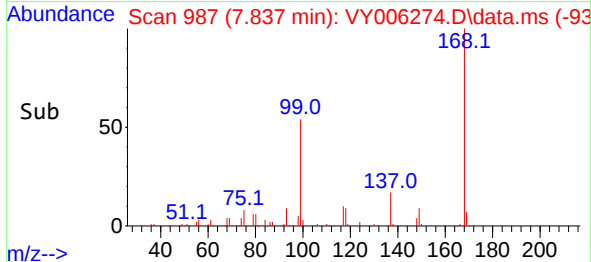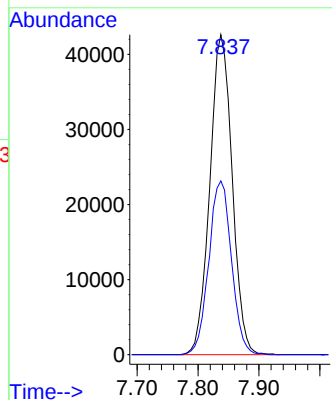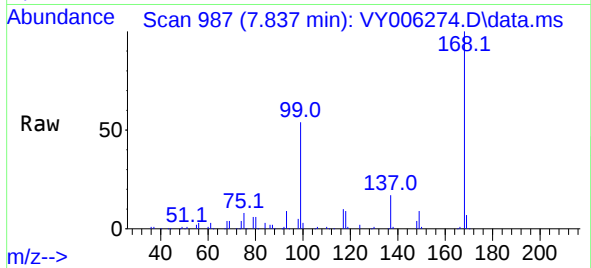

#16
Acetone
Concen: 1.053 ug/l
RT: 4.058 min Scan# 367
Delta R.T. 0.103 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22


Tgt Ion: 43 Resp: 342
Ion Ratio Lower Upper
43 100
58 0.0 22.0 33.0#

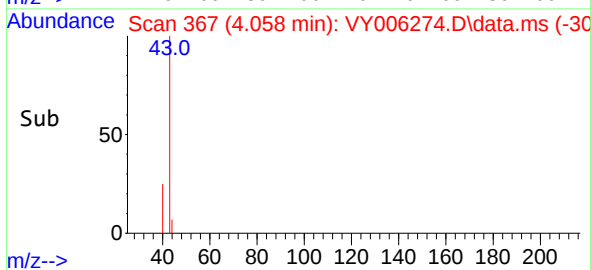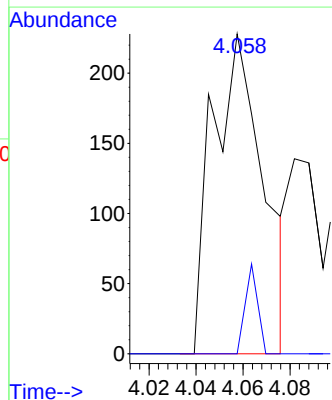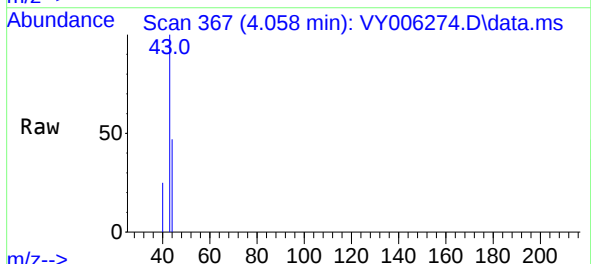



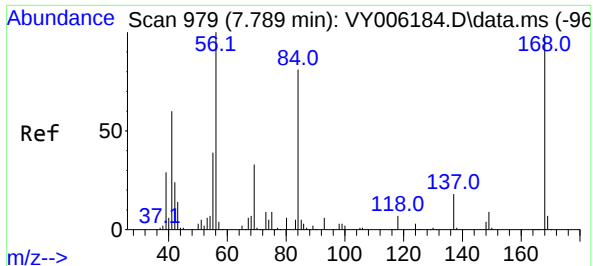


#31
Cyclohexane
Concen: 1.208 ug/l
RT: 7.837 min Scan# 987
Delta R.T. 0.049 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01



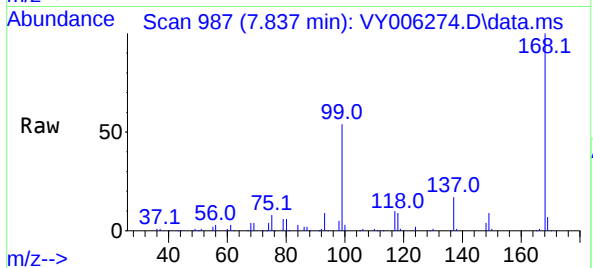



Tgt Ion: 56 Resp: 2662
Ion Ratio Lower Upper
56 100
69 142.4 26.7 40.1#
84 100.6 67.2 100.8

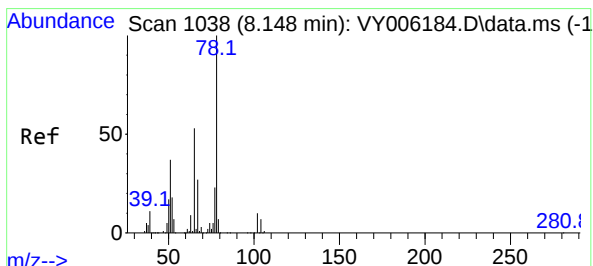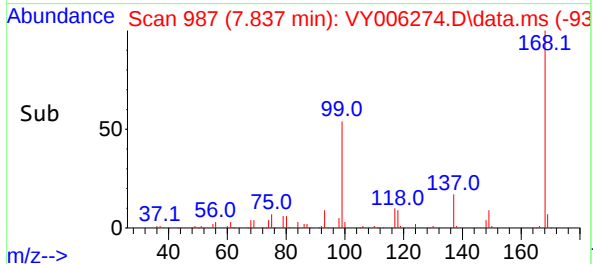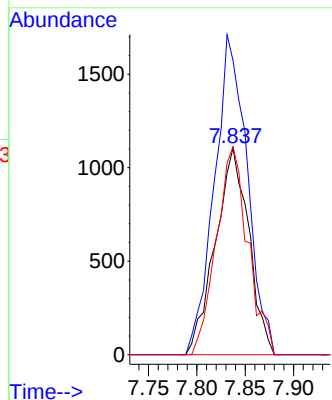

#33
1,2-Dichloroethane-d4
Concen: 52.677 ug/l
RT: 8.179 min Scan# 1043
Delta R.T. 0.030 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion: 65 Resp: 61282
Ion Ratio Lower Upper
65 100
67 49.1 0.0 99.4

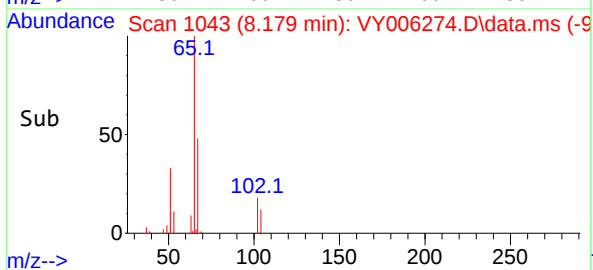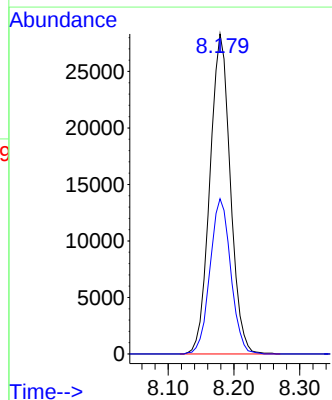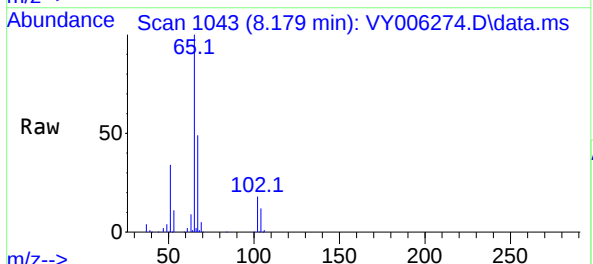




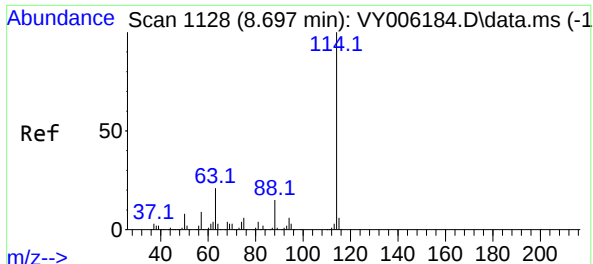


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.721 min Scan# 1132
Delta R.T. 0.024 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01




Tgt Ion:	114	Resp:	172296
Ion	Ratio	Lower	Upper
114	100		
63	21.1	0.0	43.2
88	14.6	0.0	31.8

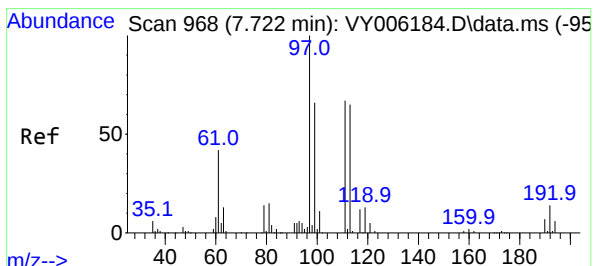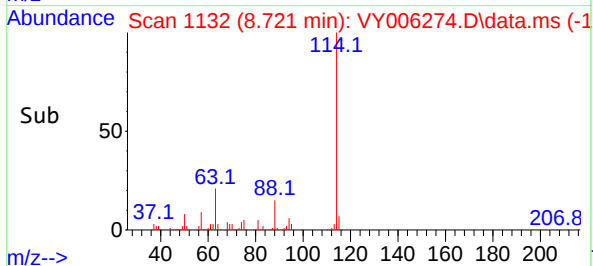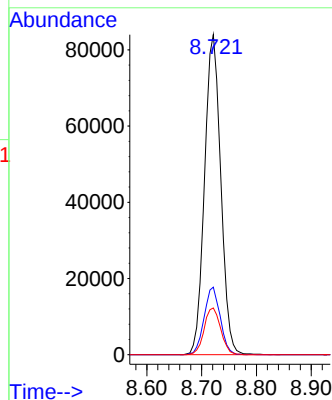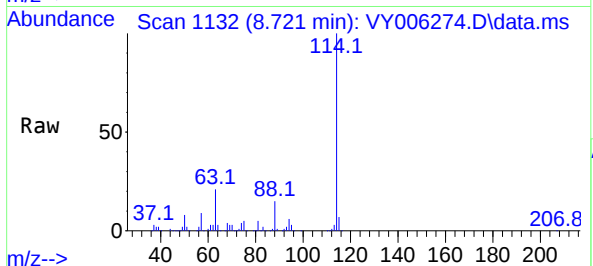


#35

Dibromofluoromethane
Concen: 47.958 ug/l
RT: 7.758 min Scan# 974
Delta R.T. 0.036 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion:	113	Resp:	44146
Ion	Ratio	Lower	Upper
113	100		
111	104.4	82.6	124.0
192	24.0	17.6	26.4

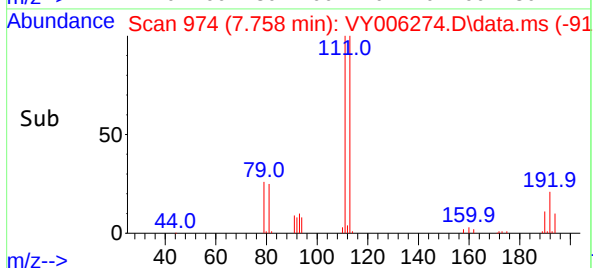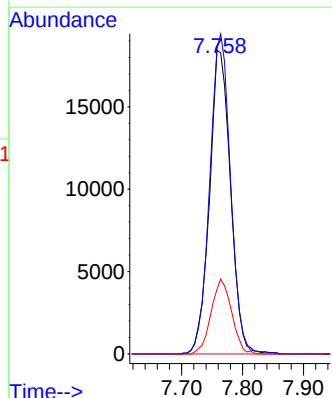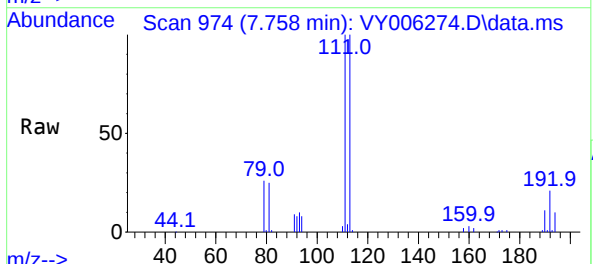




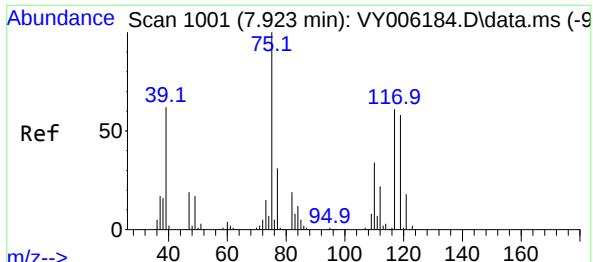


#36

1,1-Dichloropropene
Concen: 4.902 ug/l
RT: 7.837 min Scan# 987
Delta R.T. -0.086 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01




Tgt Ion: 75 Resp: 8403
Ion Ratio Lower Upper
75 100
110 10.5 17.1 51.2#
77 0.0 24.4 36.6#

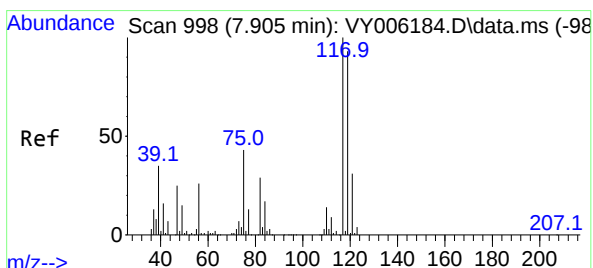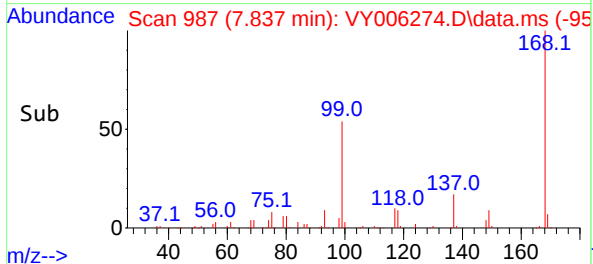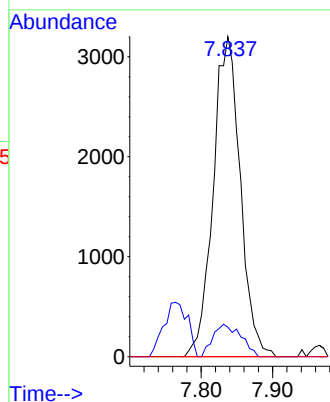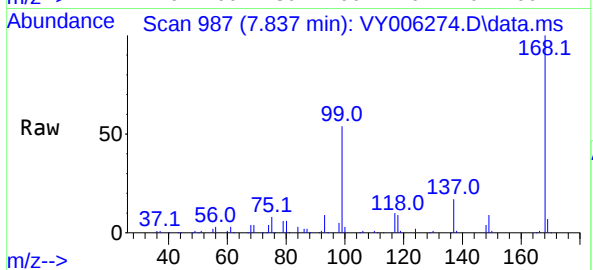


#38

Carbon Tetrachloride
Concen: 5.885 ug/l
RT: 7.837 min Scan# 987
Delta R.T. -0.067 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion: 117 Resp: 10652
Ion Ratio Lower Upper
117 100
119 5.1 77.9 116.9#
121 0.0 24.8 37.2#


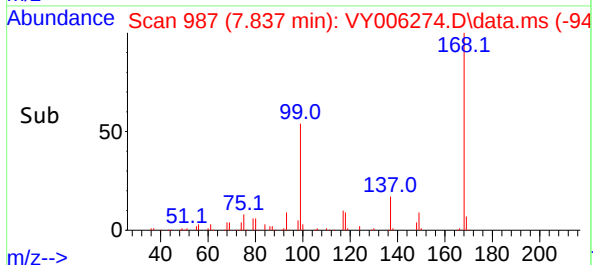
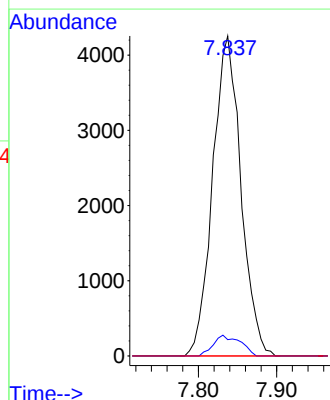
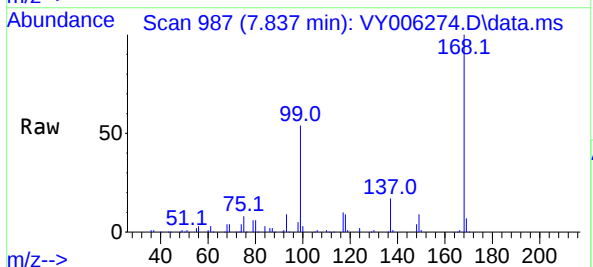


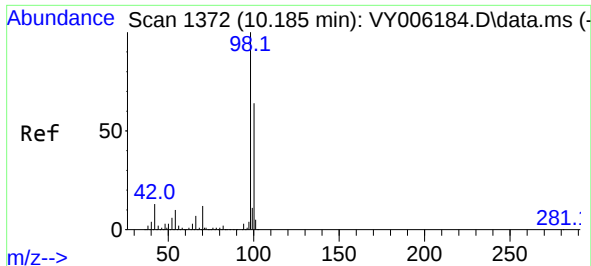

#50
Toluene-d8
Concen: 45.434 ug/l
RT: 10.197 min Scan# 1374
Delta R.T. 0.012 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22




Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01


Tgt Ion: 98 Resp: 175036
Ion Ratio Lower Upper
98 100
100 64.2 50.2 75.2

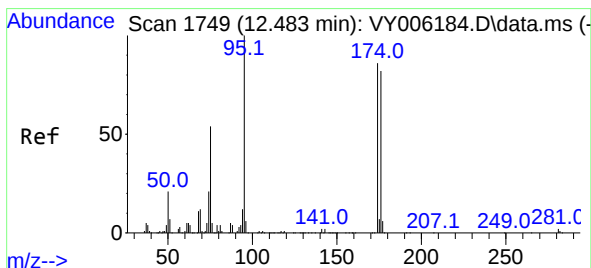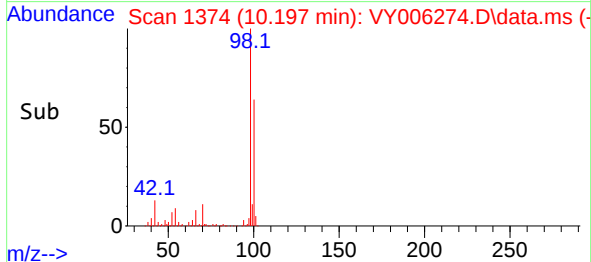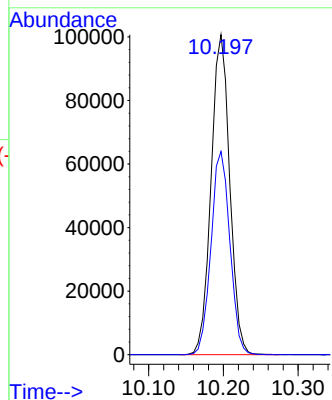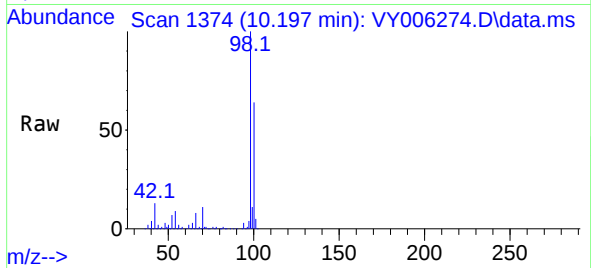

#62
4-Bromofluorobenzene
Concen: 44.655 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion: 95 Resp: 58442
Ion Ratio Lower Upper
95 100
174 95.3 0.0 177.0
176 90.2 0.0 175.8


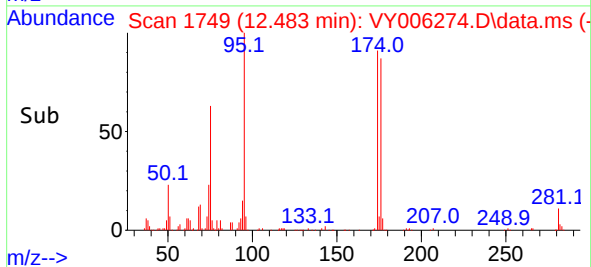
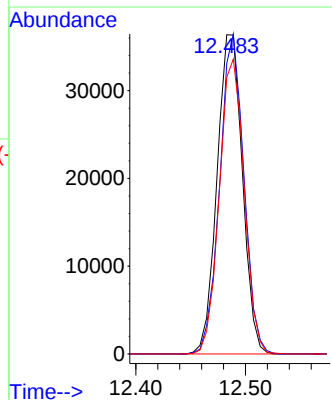
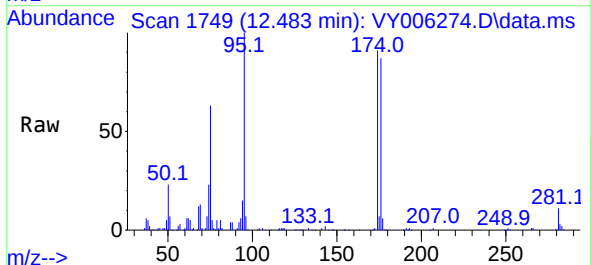


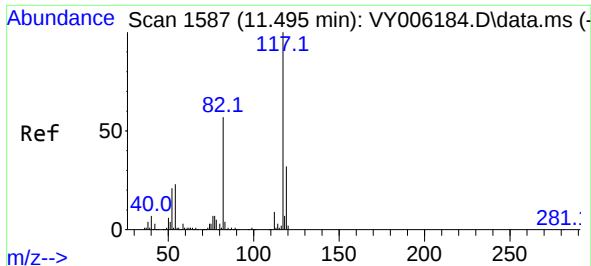

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.501 min Scan# 1588
Delta R.T. 0.006 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22




Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01

Tgt Ion:	117	Resp:	154158
Ion	Ratio	Lower	Upper
117	100		
82	53.2	43.0	64.4
119	32.2	25.4	38.0

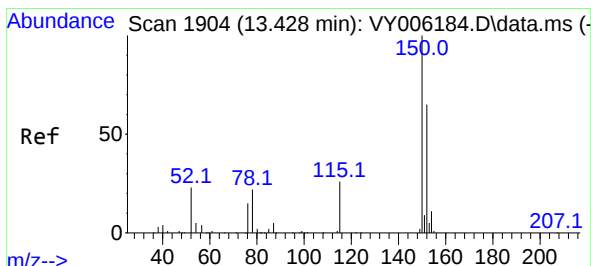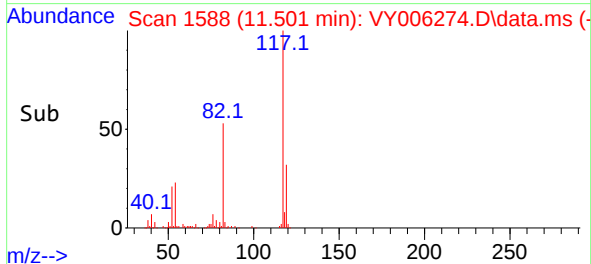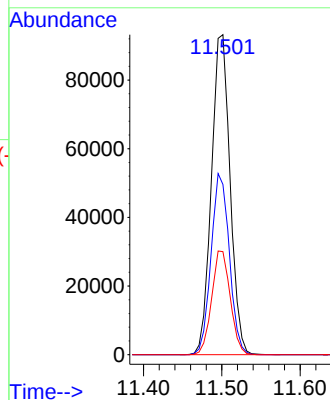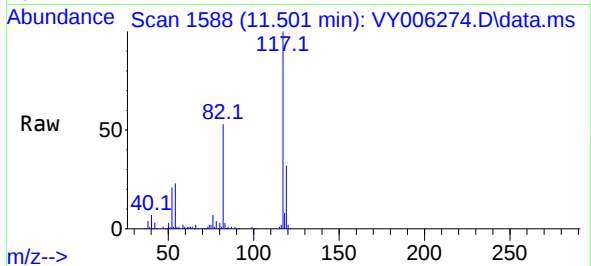


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22


Tgt Ion:	152	Resp:	79699
Ion	Ratio	Lower	Upper
152	100		
115	55.8	28.2	84.7
150	158.3	0.0	347.6

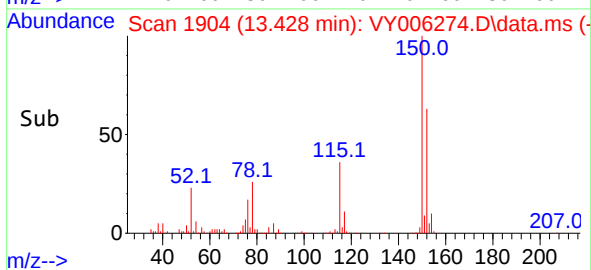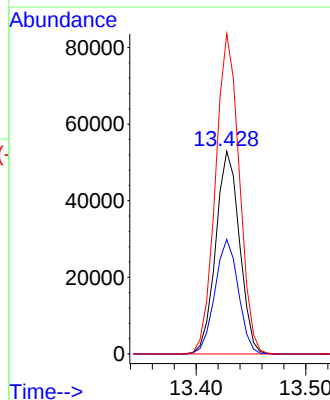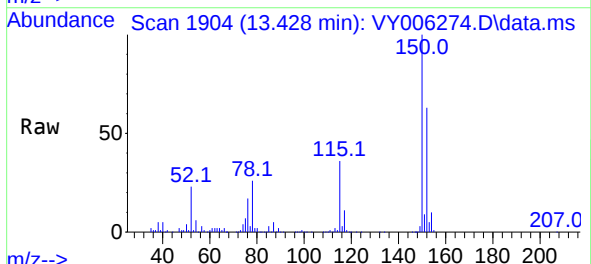


Abundance Scan 1774 (12.635 min): VY006184.D\data.ms (-

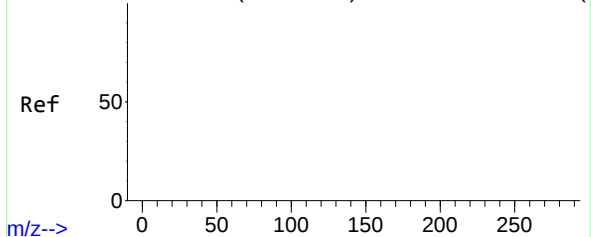


m/z--> Scan 1749 (12.483 min): VY006274.D\data.ms (-

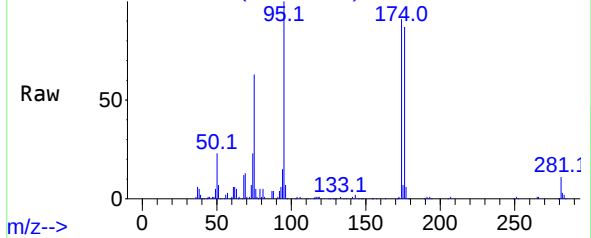


Abundance Scan 1749 (12.483 min): VY006274.D\data.ms (-

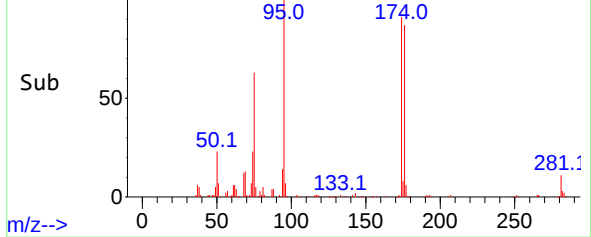


m/z--> Scan 1732 (12.379 min): VY006184.D\data.ms (-

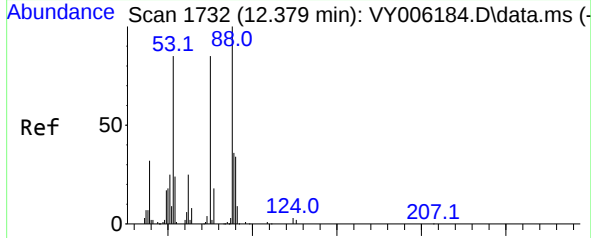

m/z--> Scan 1749 (12.483 min): VY006274.D\data.ms (-

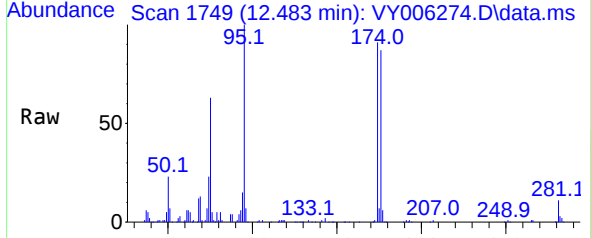


Abundance Scan 1749 (12.483 min): VY006274.D\data.ms (-

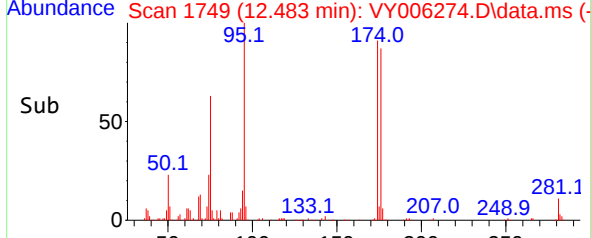

m/z--> Scan 1749 (12.483 min): VY006274.D\data.ms (-


#76
1,2,3-Trichloropropane
Concen: 44.187 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.153 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion: 75 Resp: 34229
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#

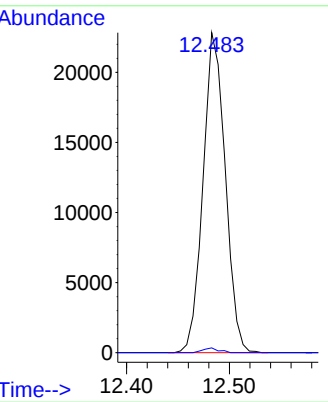

#81
trans-1,4-Dichloro-2-butene
Concen: 86.834 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.103 min
Lab File: VY006274.D
Acq: 04 Oct 2021 14:22

Tgt Ion: 75 Resp: 34229
Ion Ratio Lower Upper
75 100
53 0.0 85.3 127.9#
89 0.1 37.0 55.4#

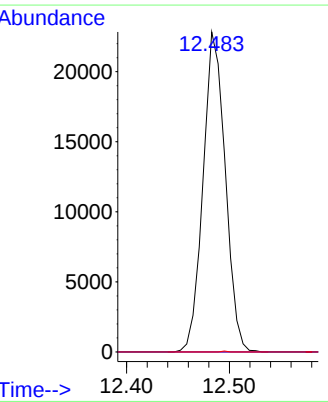

Instrument :
MSVOA_Y
ClientSampleId :
VY1004SBL01