
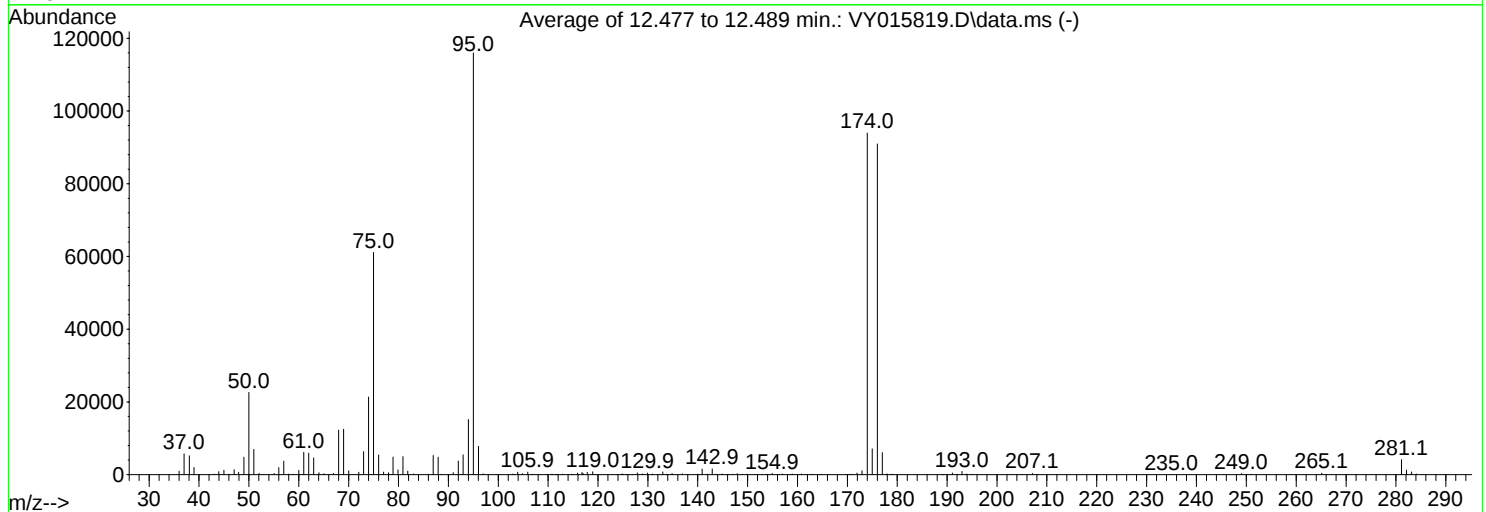


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100423\
Data File : VY015819.D
Acq On : 04 Oct 2023 08:52
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
Title : SW846 8260
Last Update : Wed Sep 20 01:39:40 2023

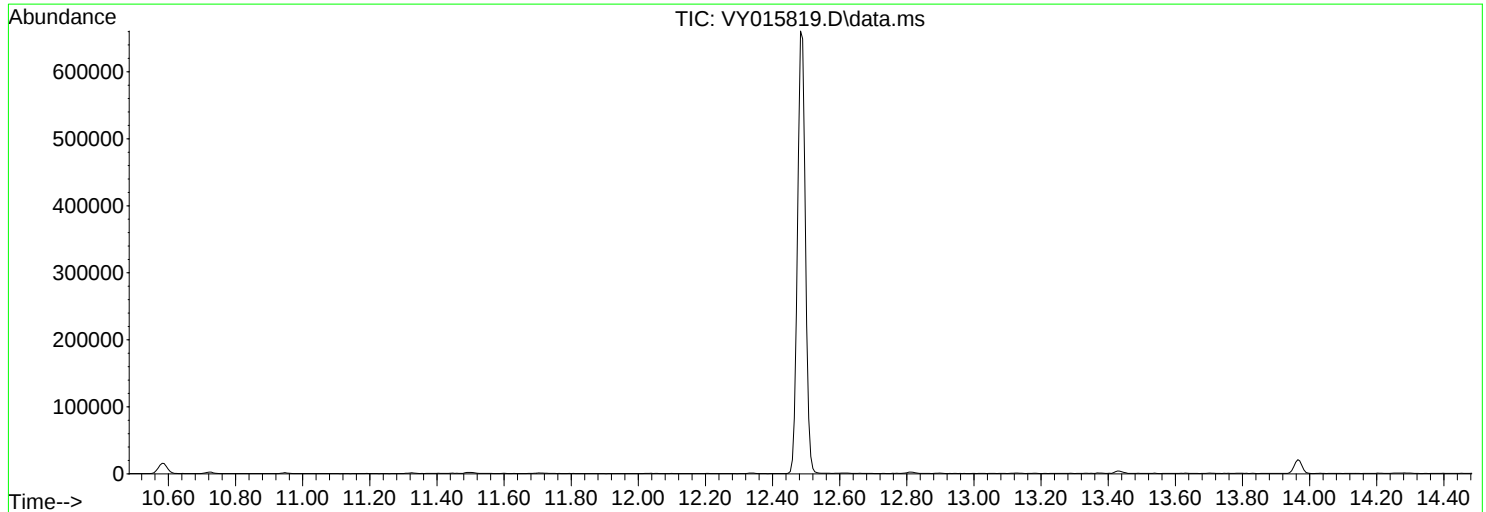

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	22613	PASS
75	95	30	60	52.7	61112	PASS
95	95	100	100	100.0	116000	PASS
96	95	5	9	6.7	7771	PASS
173	174	0.00	2	1.1	1043	PASS
174	95	50	100	81.0	93939	PASS
175	174	5	9	7.5	7079	PASS
176	174	95	101	96.8	90952	PASS
177	176	5	9	6.7	6055	PASS