


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv100520\
Data File : VY003452.D
Acq On : 05 Oct 2020 13:59
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y100520S.M
Title : SW846 8260
Last Update : Tue Oct 06 04:23:24 2020

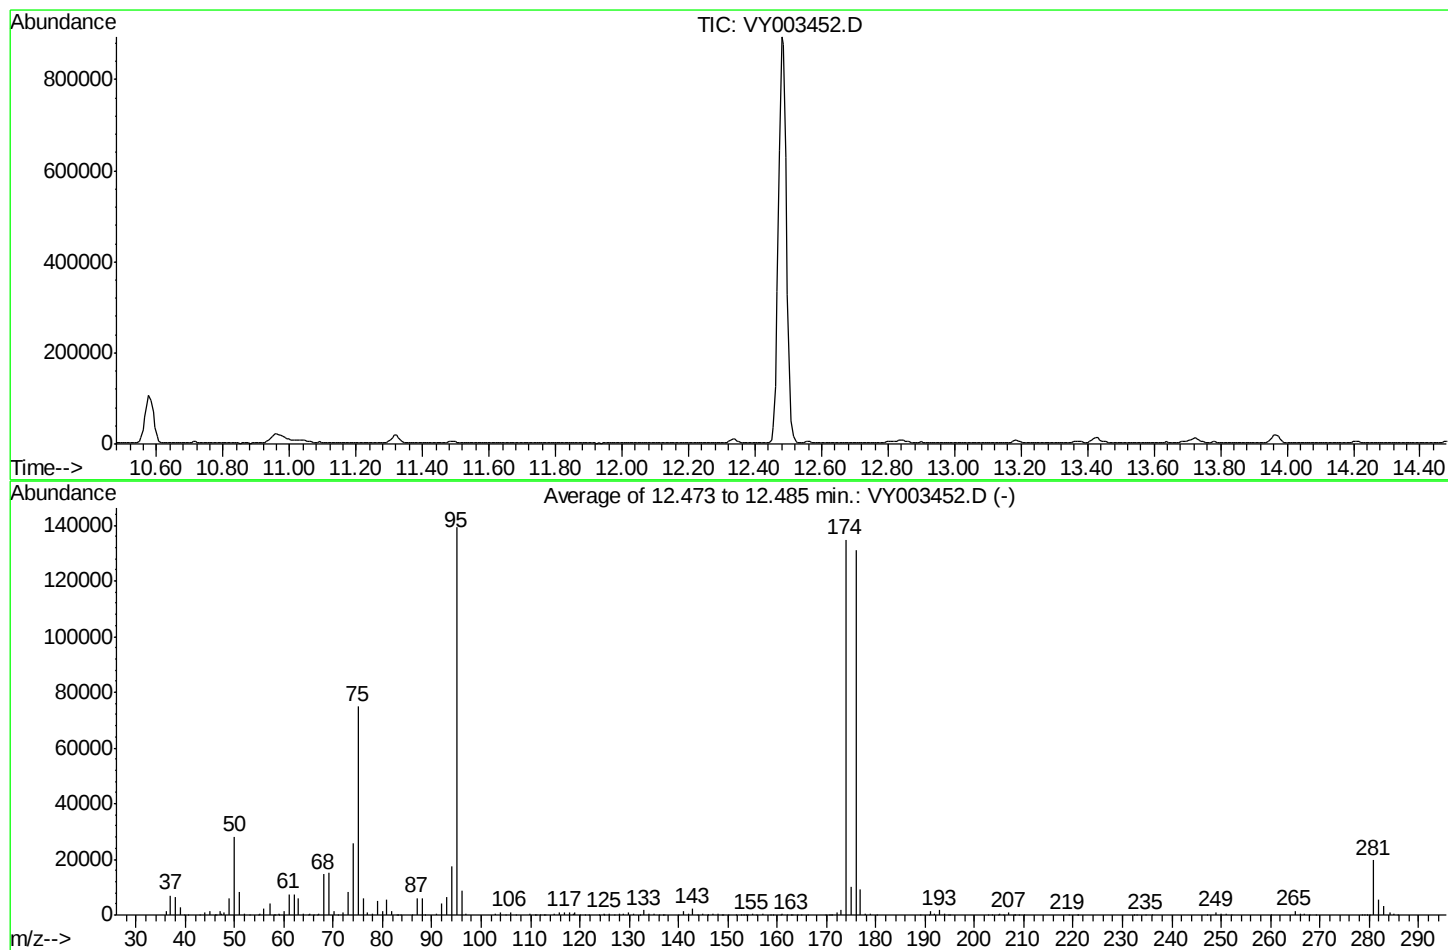

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	28130	PASS
75	95	30	60	53.7	74805	PASS
95	95	100	100	100.0	139272	PASS
96	95	5	9	6.4	8897	PASS
173	174	0.00	2	1.3	1808	PASS
174	95	50	100	96.9	134960	PASS
175	174	5	9	7.7	10351	PASS
176	174	95	101	97.0	130869	PASS
177	176	5	9	7.1	9323	PASS