

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY100623\  
 Data File : VY015862.D  
 Acq On : 06 Oct 2023 15:11  
 Operator : SY/MD  
 Sample : 04765-03  
 Misc : 5.01g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 TT-2

Quant Time: Oct 07 07:27:39 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y100523S.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Oct 06 05:54:04 2023  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.789  | 168  | 221638   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 392912   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.489 | 117  | 361053   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.422 | 152  | 166422   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.136  | 65    | 146727   | 67.289   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 134.580% |
| 35) Dibromofluoromethane    | 7.716  | 113   | 127097   | 56.750   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 113.500% |
| 50) Toluene-d8              | 10.179 | 98    | 457597   | 62.931   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 58 - 134 | Recovery | =    | 125.860% |
| 62) 4-Bromofluorobenzene    | 12.483 | 95    | 156945   | 52.804   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 30 - 143 | Recovery | =    | 105.600% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY100623\  
Data File : VY015862.D  
Acq On : 06 Oct 2023 15:11  
Operator : SY/MD  
Sample : 04765-03  
Misc : 5.01g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
TT-2

Quant Time: Oct 07 07:27:39 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y100523S.M  
Quant Title : SW846 8260  
QLast Update : Fri Oct 06 05:54:04 2023  
Response via : Initial Calibration




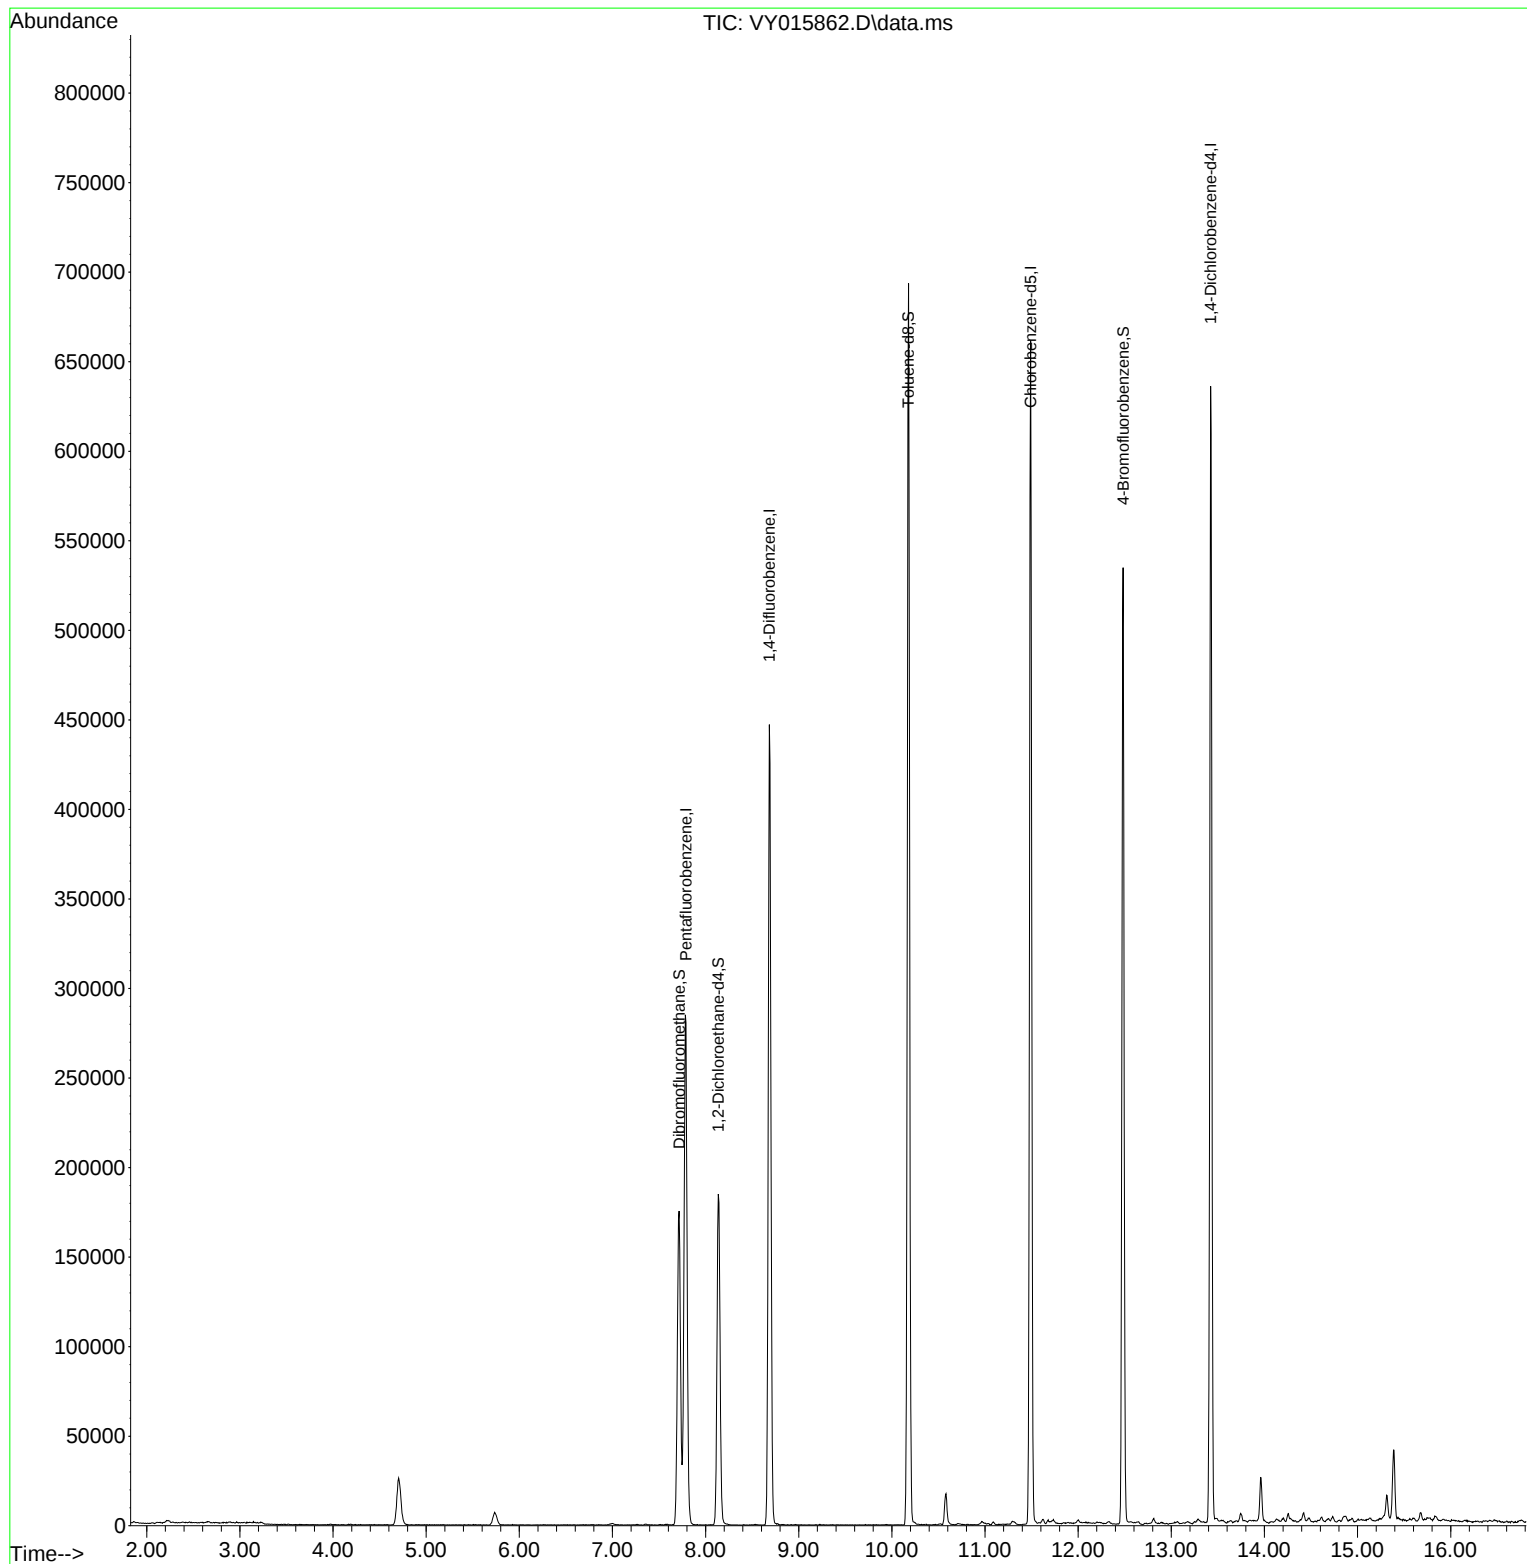


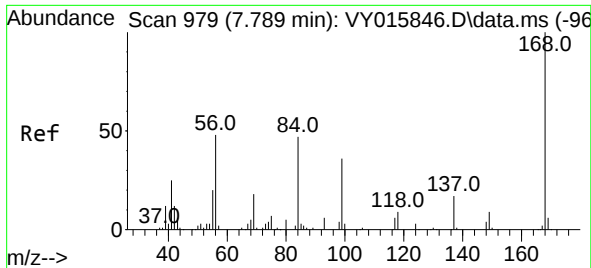

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.789 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY015862.D  
Acq: 06 Oct 2023 15:11




Instrument :  
MSVOA\_Y  
ClientSampleId :  
TT-2


Tgt Ion:168 Resp: 221638  
Ion Ratio Lower Upper  
168 100  
99 53.6 43.4 65.0

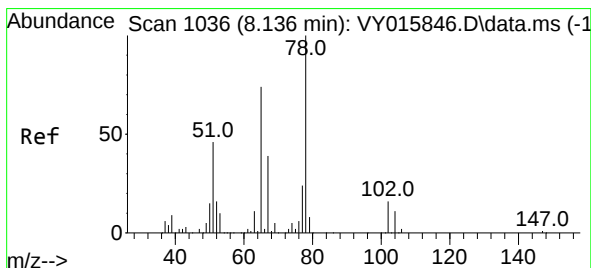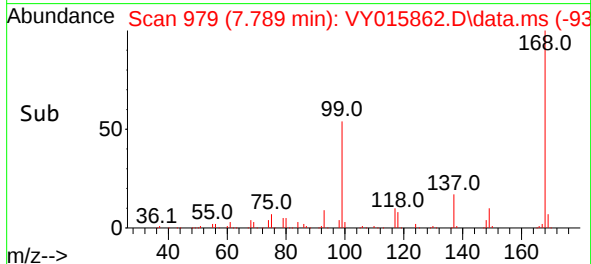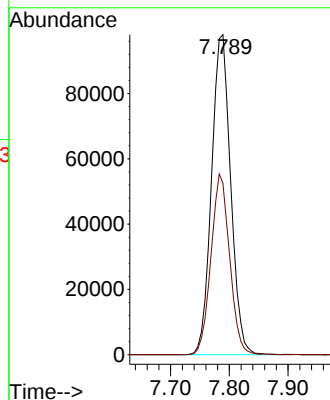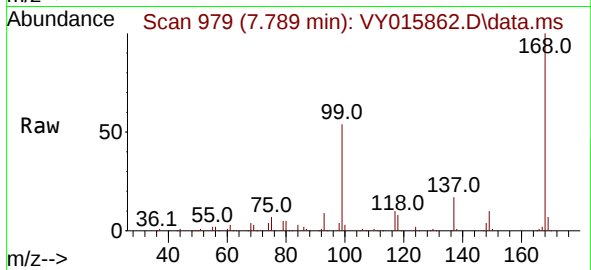

#33  
1,2-Dichloroethane-d4  
Concen: 67.289 ug/l  
RT: 8.136 min Scan# 1036  
Delta R.T. 0.000 min  
Lab File: VY015862.D  
Acq: 06 Oct 2023 15:11

Tgt Ion: 65 Resp: 146727  
Ion Ratio Lower Upper  
65 100  
67 54.3 0.0 101.8

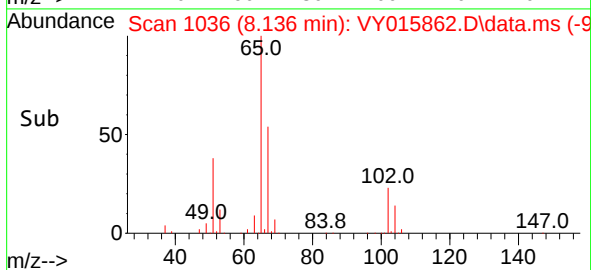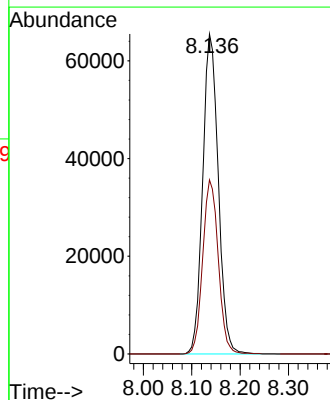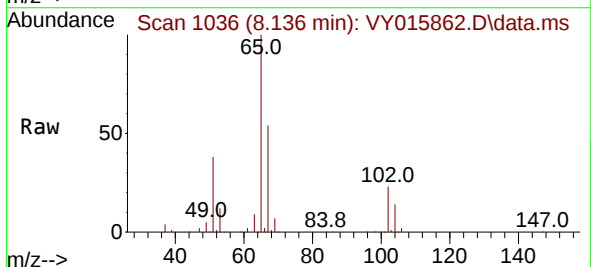

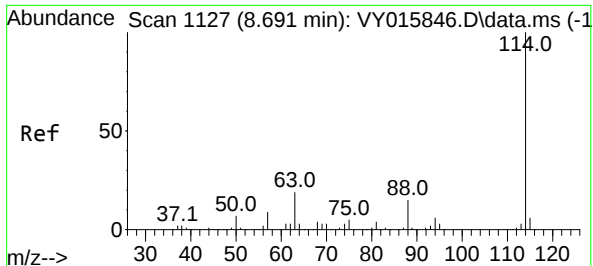

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY015862.D

Acq: 06 Oct 2023 15:11

Instrument :

MSVOA\_Y

ClientSampleId :

TT-2





Tgt Ion:114 Resp: 392912

Ion Ratio Lower Upper

114 100

63 19.6 0.0 42.4

88 15.4 0.0 30.6

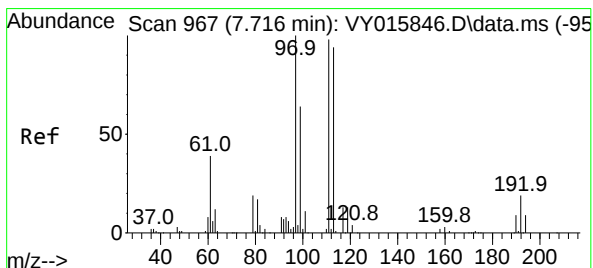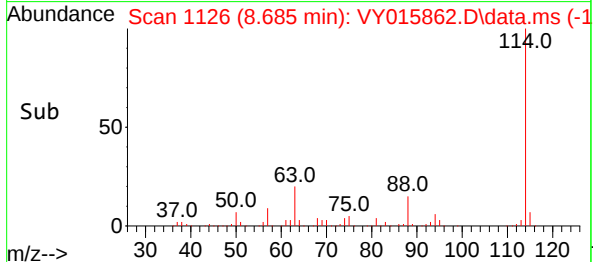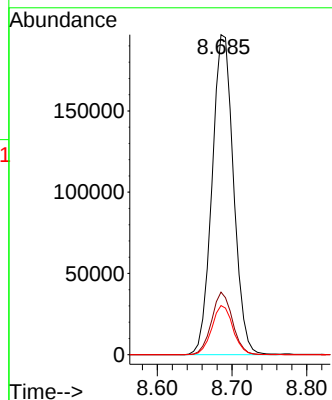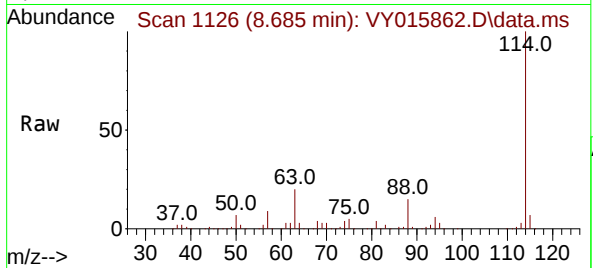

#35

Dibromofluoromethane

Concen: 56.750 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY015862.D

Acq: 06 Oct 2023 15:11




Tgt Ion:113 Resp: 127097


Ion Ratio Lower Upper

113 100

111 102.2 81.3 121.9

192 19.2 16.9 25.3


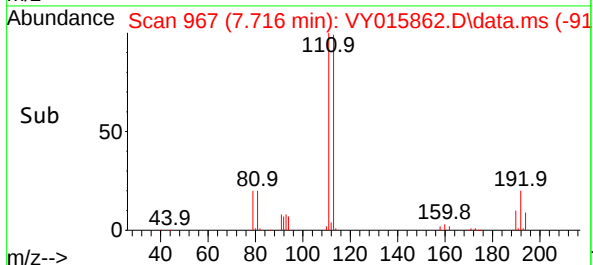
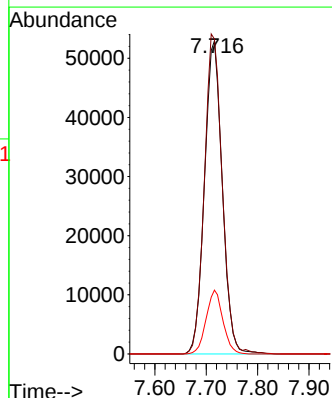
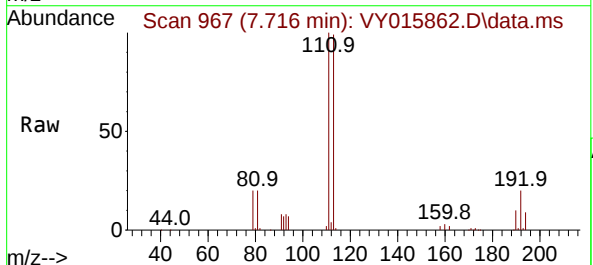


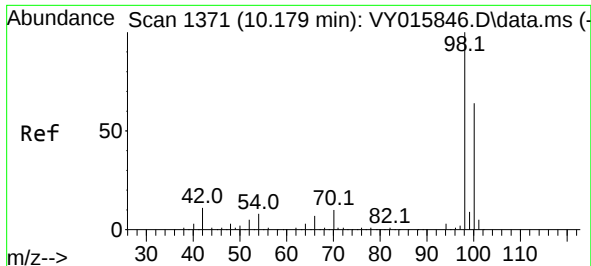

#50  
Toluene-d8  
Concen: 62.931 ug/l  
RT: 10.179 min Scan# 1371  
Delta R.T. 0.000 min  
Lab File: VY015862.D  
Acq: 06 Oct 2023 15:11




Instrument :  
MSVOA\_Y  
ClientSampleId :  
TT-2


Tgt Ion: 98 Resp: 457597  
Ion Ratio Lower Upper  
98 100  
100 65.3 50.1 75.1

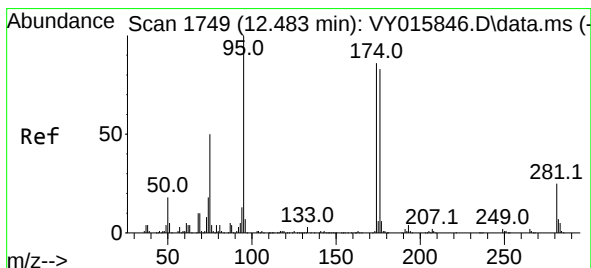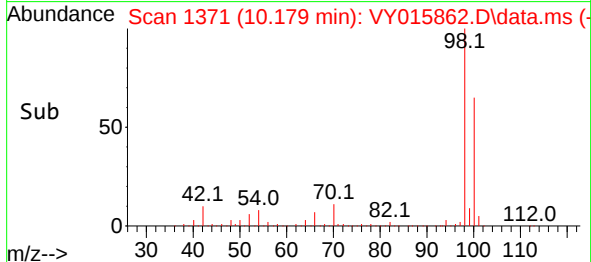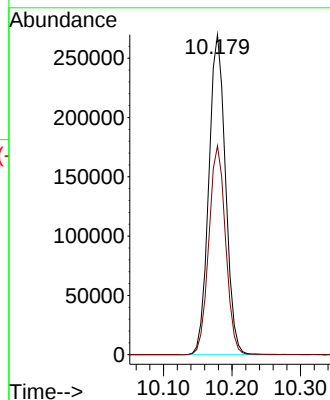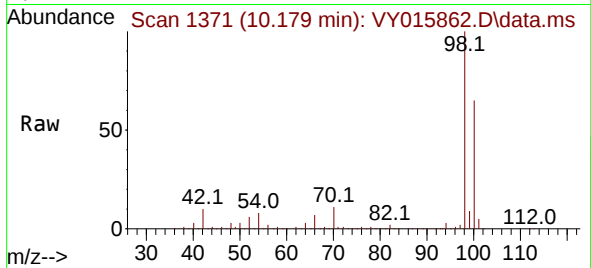

#62  
4-Bromofluorobenzene  
Concen: 52.804 ug/l  
RT: 12.483 min Scan# 1749  
Delta R.T. 0.000 min  
Lab File: VY015862.D  
Acq: 06 Oct 2023 15:11

Tgt Ion: 95 Resp: 156945  
Ion Ratio Lower Upper  
95 100  
174 84.6 0.0 178.2  
176 82.4 0.0 173.8

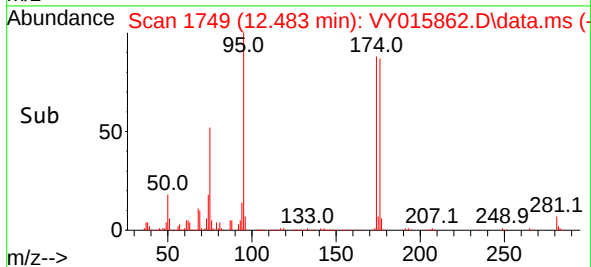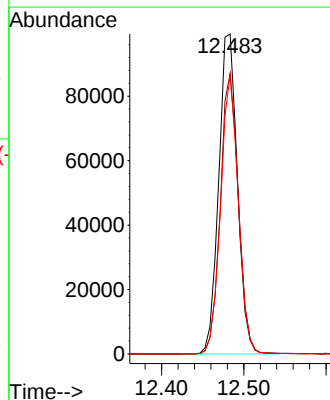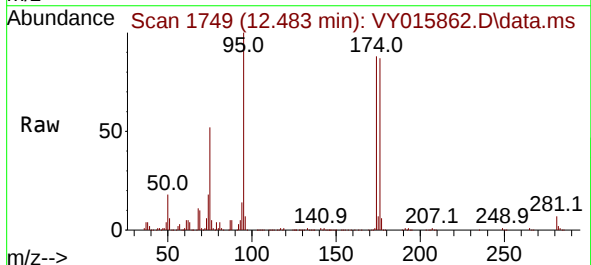

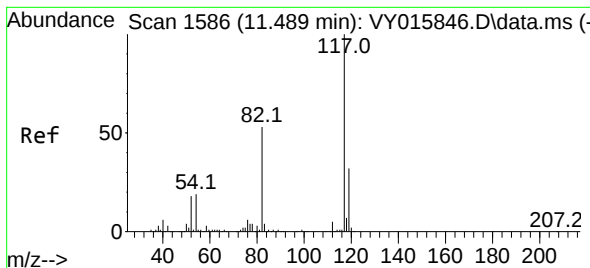

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY015862.D

Acq: 06 Oct 2023 15:11

Instrument :

MSVOA\_Y

ClientSampleId :

TT-2





Tgt Ion:117 Resp: 361053

Ion Ratio Lower Upper

117 100

82 54.2 43.4 65.0

119 32.1 26.3 39.5

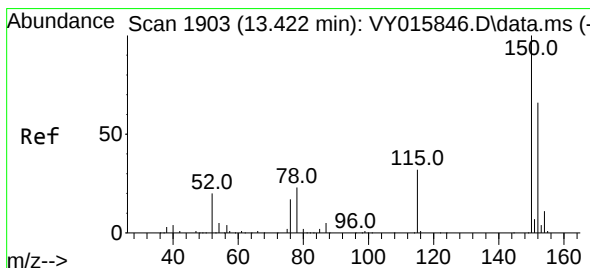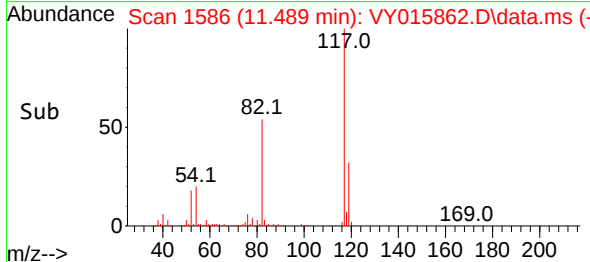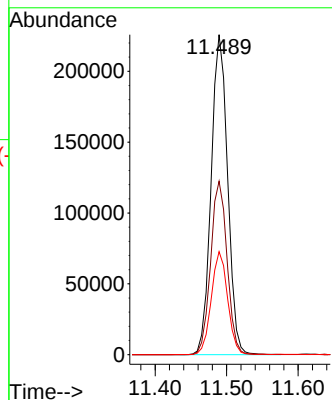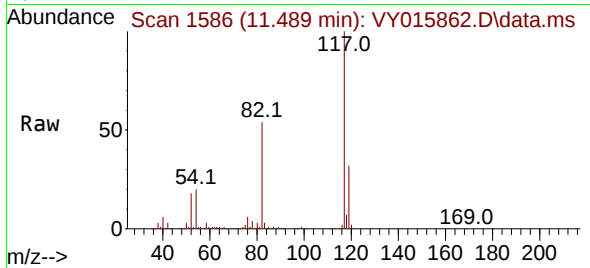

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY015862.D

Acq: 06 Oct 2023 15:11

Tgt Ion:152 Resp: 166422

Ion Ratio Lower Upper

152 100

115 58.4 28.8 86.5

150 157.5 0.0 348.8

