
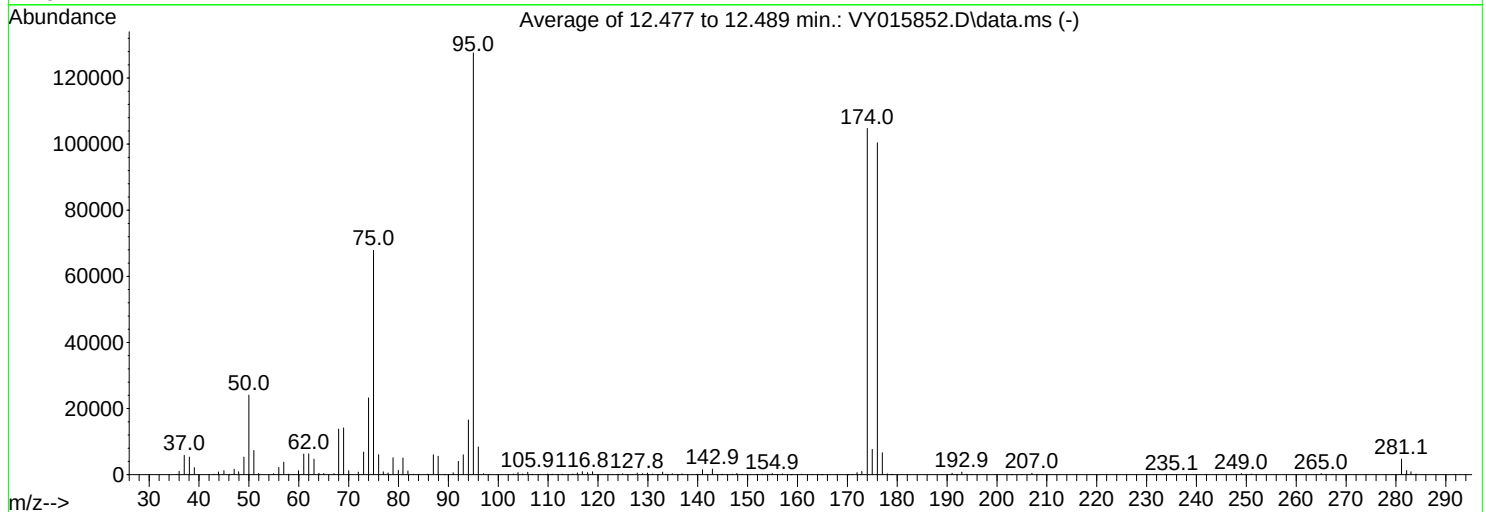


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY100623\  
Data File : VY015852.D  
Acq On : 06 Oct 2023 08:49  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y100523S.M  
Title : SW846 8260  
Last Update : Fri Oct 06 05:54:04 2023

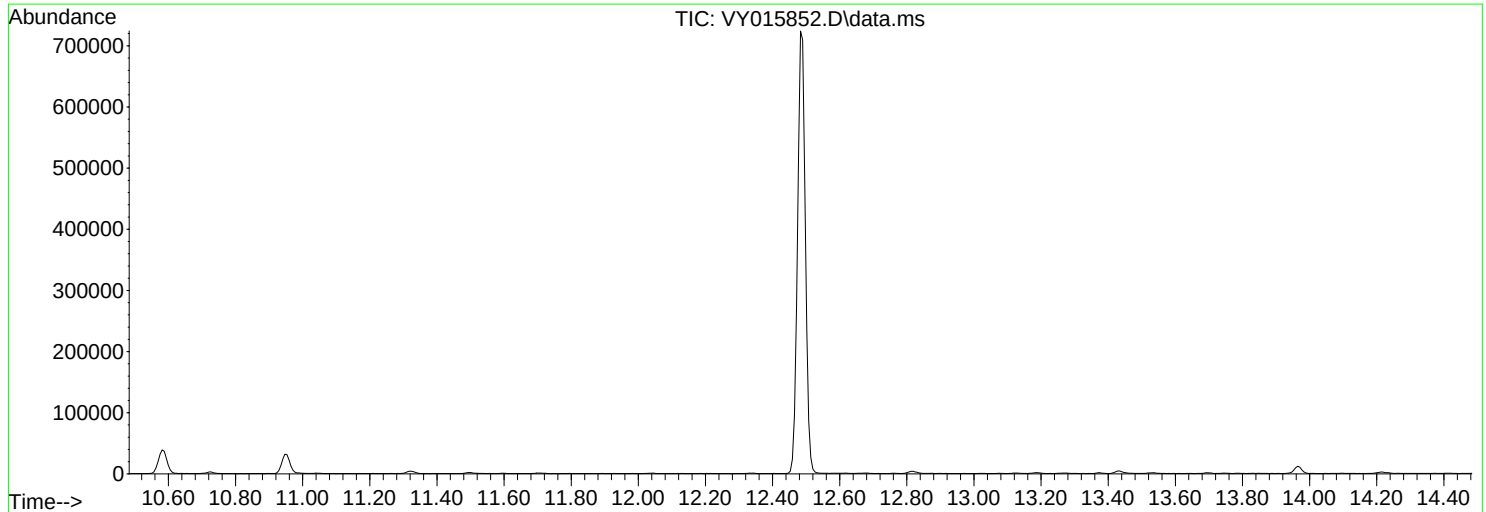

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.8  | 24051  | PASS      |
| 75     | 95      | 30     | 60     | 53.2  | 67899  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 127624 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 8369   | PASS      |
| 173    | 174     | 0.00   | 2      | 0.9   | 963    | PASS      |
| 174    | 95      | 50     | 100    | 82.1  | 104749 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 7674   | PASS      |
| 176    | 174     | 95     | 101    | 95.8  | 100392 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 6639   | PASS      |