
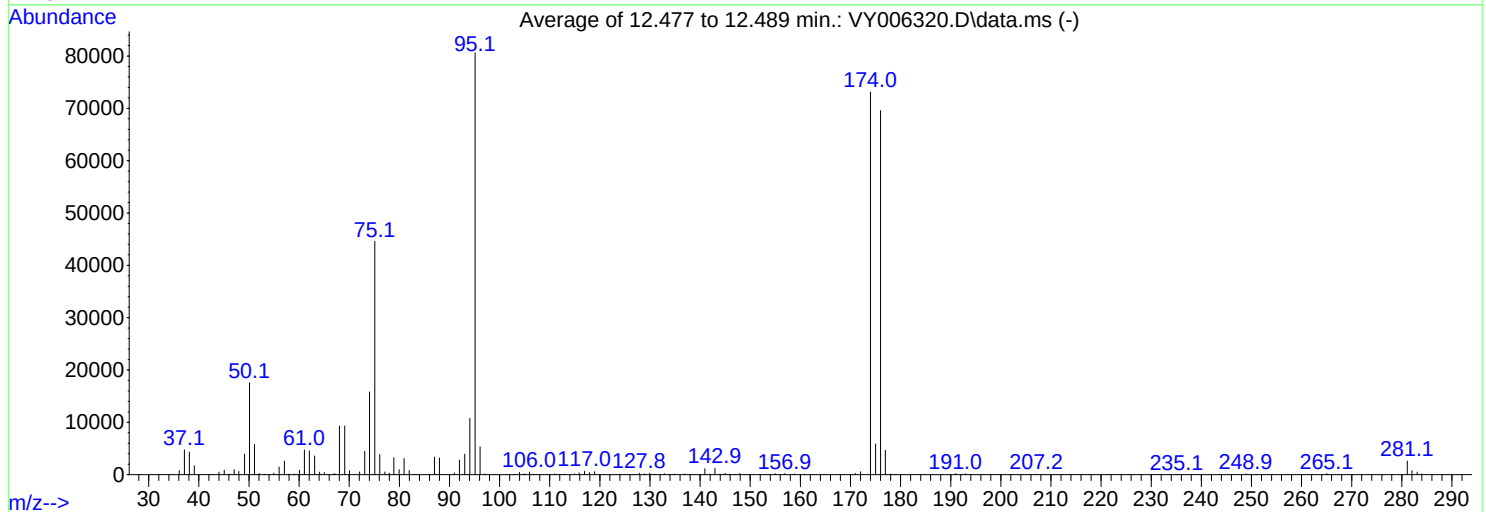


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100721\
 Data File : VY006320.D
 Acq On : 07 Oct 2021 08:01
 Operator : SY/MD
 Sample : BFB806
 Misc : 5.00G/10ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB806

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL100521SMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 09 00:39:56 2021

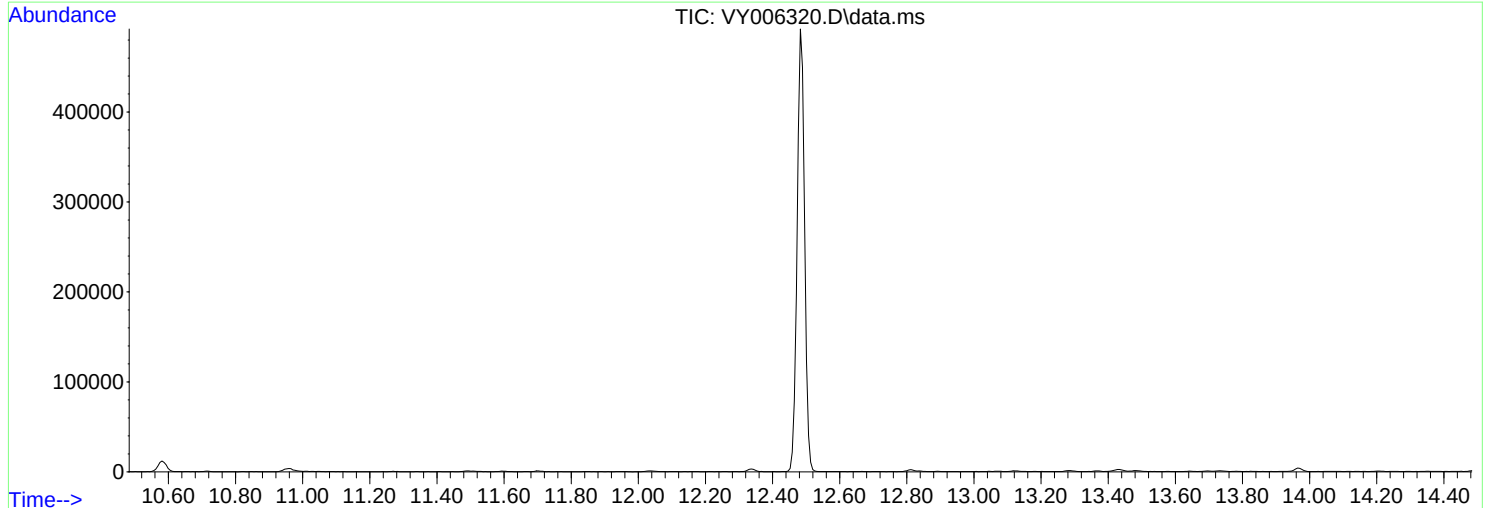

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17545	PASS
75	95	30	80	55.3	44573	PASS
95	95	100	100	100.0	80608	PASS
96	95	5	9	6.6	5312	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.7	73096	PASS
175	174	5	9	8.1	5885	PASS
176	174	95	105	95.2	69560	PASS
177	176	5	10	6.7	4656	PASS

Scan 1741 (12.434 min): VY006320.D\data.ms
BFB806

m/z	Abundance
40.00	94.0
44.00	154.0
207.00	94.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

m/z	Abundance
36.10	636.0
37.10	4461.0
38.10	4203.0
39.10	1891.0
40.00	232.0
44.00	553.0
45.10	815.0
46.10	86.0
47.10	766.0
48.00	531.0
49.10	3438.0
50.10	15858.0
51.10	5057.0
52.10	195.0
53.10	51.0
54.90	232.0
56.00	1280.0
57.00	2538.0
58.90	97.0
60.10	724.0
61.10	4171.0
62.10	4239.0
63.10	3385.0
64.10	519.0
65.00	508.0
66.90	167.0
67.20	198.0
68.00	8329.0
69.10	8303.0
70.10	696.0
72.00	392.0
73.10	4013.0
74.10	13958.0
75.10	39688.0
76.10	3638.0
77.20	526.0
77.80	306.0
78.90	2926.0
80.00	789.0
80.90	2808.0
82.00	701.0
83.10	73.0
86.20	152.0
87.00	2702.0
88.00	2864.0
91.00	326.0
92.00	2373.0
93.00	3399.0
94.00	9226.0
95.10	71160.0
96.10	4725.0
97.10	151.0
102.90	53.0
103.90	350.0
105.00	122.0
106.00	417.0
106.90	63.0
109.90	63.0
110.90	93.0
113.00	55.0
115.00	85.0
115.80	319.0
116.90	561.0
117.90	312.0
118.90	553.0
127.90	189.0
128.90	172.0
129.90	298.0
130.80	66.0
132.90	99.0
133.70	88.0
134.90	163.0
136.80	139.0
139.80	65.0
141.00	874.0
141.90	118.0
143.00	1049.0
144.00	78.0
145.00	281.0
145.80	131.0
147.90	174.0
148.90	63.0
149.70	107.0
154.00	89.0
155.00	166.0
156.90	188.0
159.00	74.0
171.00	189.0
172.00	484.0
174.00	59128.0
175.00	4639.0
176.00	55648.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

177.00	3986.0
177.90	195.0
191.00	86.0
192.90	88.0
207.20	153.0
265.10	121.0
281.10	1077.0
282.00	447.0
283.10	183.0
284.00	73.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

m/z	Abundance
36.10	896.0
37.10	5592.0
38.10	4683.0
39.10	1748.0
40.00	157.0
44.10	795.0
45.00	973.0
46.10	137.0
47.10	1057.0
47.90	751.0
49.10	4338.0
50.10	20128.0
51.10	6391.0
52.00	238.0
53.10	129.0
55.00	271.0
56.00	1638.0
57.00	2896.0
57.90	163.0
59.00	78.0
60.00	960.0
61.00	5293.0
62.10	5052.0
63.10	3898.0
64.10	540.0
65.00	437.0
67.00	256.0
68.00	10563.0
69.10	10666.0
70.10	890.0
72.10	615.0
73.10	4899.0
74.00	17632.0
75.10	49976.0
76.10	4073.0
77.10	586.0
78.00	485.0
78.90	3475.0
79.90	1079.0
81.00	3468.0
81.90	1007.0
83.00	85.0
85.90	96.0
87.00	3802.0
88.00	3678.0
90.80	370.0
92.00	3102.0
93.10	4266.0
94.00	12211.0
95.10	91872.0
96.10	6321.0
97.10	193.0
102.90	69.0
104.00	536.0
105.00	168.0
106.00	631.0
106.80	158.0
110.10	124.0
110.90	80.0
111.80	96.0
112.90	147.0
114.90	144.0
115.90	391.0
117.00	700.0
117.90	418.0
119.00	737.0
124.90	100.0
125.90	64.0
126.60	53.0
127.90	334.0
128.80	194.0
130.00	248.0
131.00	118.0
133.00	143.0
133.80	83.0
135.00	173.0
137.00	199.0
139.80	57.0
140.90	1386.0
142.00	107.0
142.90	1362.0
143.90	115.0
145.00	229.0
145.80	188.0
147.10	67.0
148.00	300.0
148.90	87.0
149.90	76.0
154.00	84.0
154.90	265.0
156.90	240.0
158.90	138.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

160.80	114.0
171.00	250.0
172.10	570.0
174.00	81024.0
175.00	6746.0
176.00	77360.0
176.90	5210.0
178.10	168.0
178.80	64.0
179.10	51.0
191.00	220.0
193.10	228.0
193.90	73.0
207.10	121.0
248.90	138.0
265.10	213.0
281.00	2539.0
282.00	811.0
282.90	483.0
284.00	179.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

m/z	Abundance
36.10	811.0
37.10	4194.0
38.10	4034.0
39.10	1497.0
40.10	103.0
42.90	76.0
44.10	552.0
45.00	823.0
46.10	85.0
47.00	1047.0
47.90	552.0
49.10	3942.0
50.10	16648.0
51.10	5906.0
52.00	192.0
54.90	161.0
55.10	159.0
56.00	1455.0
57.10	2383.0
58.00	149.0
59.10	80.0
60.00	920.0
61.00	4626.0
62.00	4396.0
63.10	3445.0
64.10	404.0
65.00	291.0
67.10	305.0
68.10	8880.0
69.10	8926.0
70.00	683.0
72.00	539.0
73.10	4533.0
74.10	15799.0
75.10	44056.0
76.10	3869.0
77.00	473.0
78.00	312.0
78.90	3336.0
80.00	949.0
80.90	3000.0
82.00	691.0
83.00	107.0
85.90	99.0
87.00	3611.0
88.00	3029.0
91.00	354.0
92.00	2866.0
93.00	4114.0
94.10	10853.0
95.10	78792.0
96.10	4890.0
97.00	138.0
103.10	116.0
104.00	398.0
104.70	139.0
105.10	168.0
105.80	417.0
106.80	77.0
110.00	72.0
110.90	185.0
111.90	71.0
112.90	112.0
115.00	178.0
115.90	352.0
116.90	683.0
118.00	510.0
118.90	476.0
123.90	59.0
125.00	80.0
125.90	62.0
127.80	340.0
128.80	144.0
130.00	295.0
131.00	165.0
132.90	287.0
133.90	114.0
134.70	204.0
136.90	165.0
139.90	80.0
140.90	1100.0
142.00	186.0
143.00	1268.0
143.90	77.0
145.00	214.0
146.00	126.0
146.90	156.0
147.80	159.0
149.00	64.0
149.90	118.0
155.00	172.0
156.90	197.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806

158.80	153.0
160.90	157.0
170.00	59.0
170.90	263.0
171.90	588.0
174.00	79136.0
175.00	6270.0
176.00	75672.0
177.00	4773.0
177.90	138.0
179.10	80.0
191.00	387.0
192.20	113.0
192.90	355.0
193.90	102.0
206.90	224.0
235.10	52.0
248.90	301.0
251.00	127.0
265.00	349.0
266.00	117.0
281.10	4189.0
282.00	1057.0
283.10	769.0
283.90	171.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB806