


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100819\
Data File : VY000217.D
Acq On : 08 Oct 2019 11:41
Operator : SY/MD
Sample : BFB
Misc : 5.0ml/MSVOA_Y/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y100819W.M
Title : SW846 8260
Last Update : Tue Oct 08 10:36:22 2019

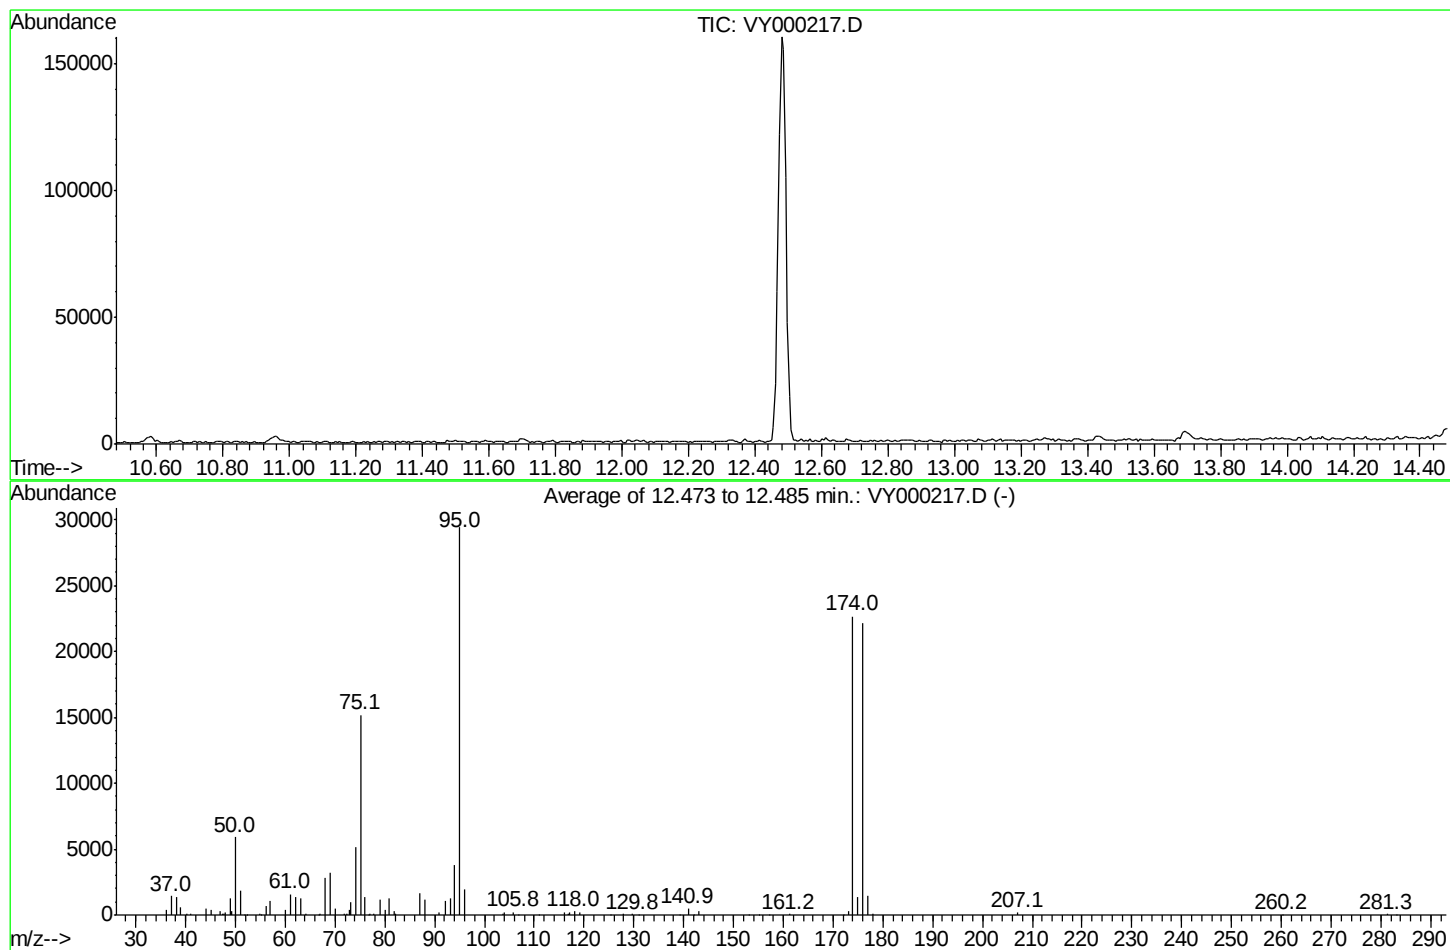

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	5924	PASS
75	95	30	60	51.6	15194	PASS
95	95	100	100	100.0	29424	PASS
96	95	5	9	6.7	1983	PASS
173	174	0.00	2	1.1	248	PASS
174	95	50	100	77.1	22685	PASS
175	174	5	9	6.1	1380	PASS
176	174	95	101	97.7	22165	PASS
177	176	5	9	6.5	1434	PASS