

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100821\
 Data File : VY006340.D
 Acq On : 07 Oct 2021 18:35
 Operator : SY/MD
 Sample : M4117-12
 Misc : 2.22G/5ML/MSVOA_Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-4(3-3.5)

Quant Time: Oct 08 07:14:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 28 17:44:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	120245	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	197743	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	183110	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	82843	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	79457	61.74	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 123.48%	
35) Dibromofluoromethane	7.728	113	59491	56.31	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 112.62%	
50) Toluene-d8	10.185	98	250738	56.71	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 113.42%	
62) 4-Bromofluorobenzene	12.483	95	74568	49.64	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 99.28%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100821\
Data File : VY006340.D
Acq On : 07 Oct 2021 18:35
Operator : SY/MD
Sample : M4117-12
Misc : 2.22G/5ML/MSVOA_Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-4(3-3.5)

Quant Time: Oct 08 07:14:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 17:44:36 2021
Response via : Initial Calibration




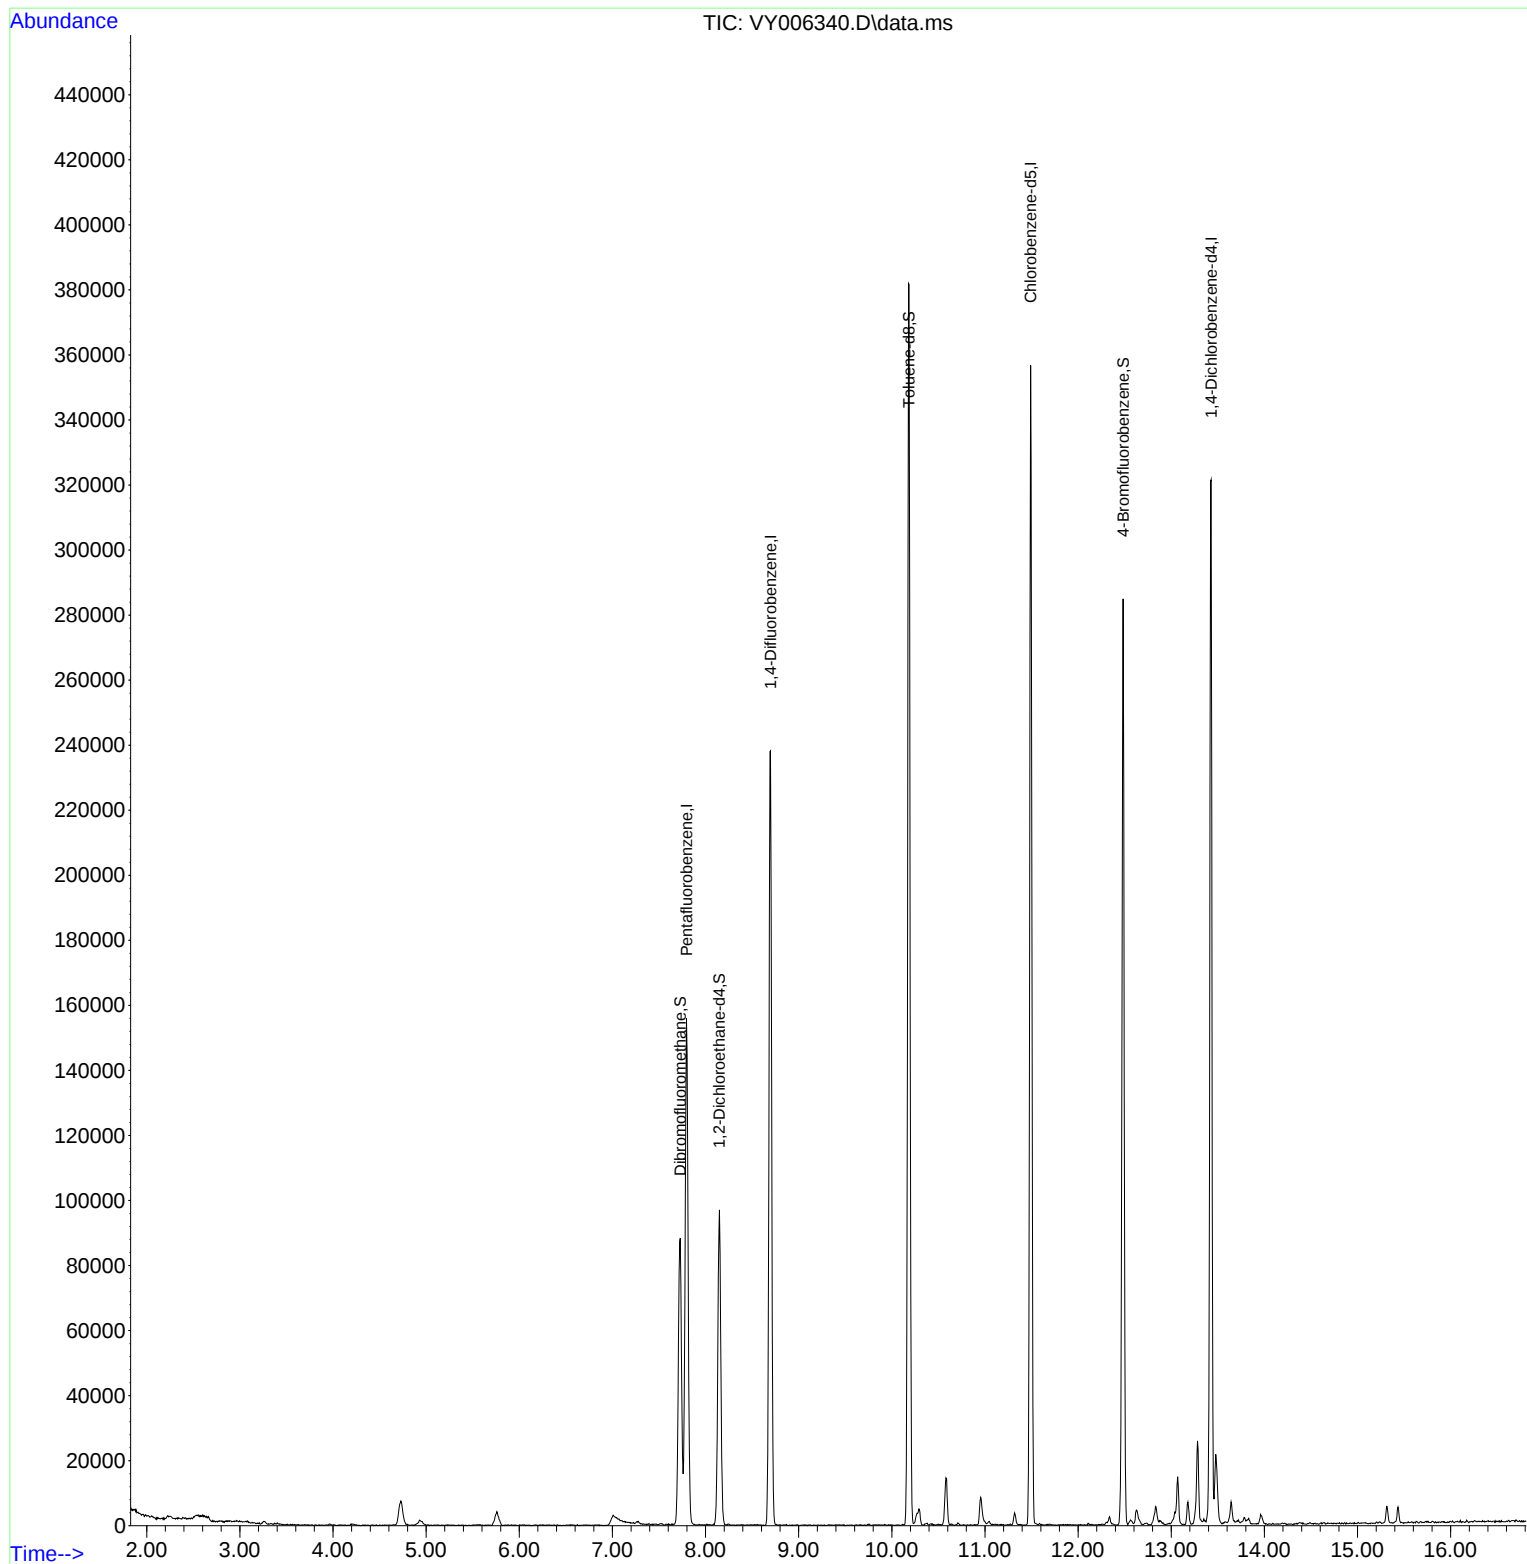


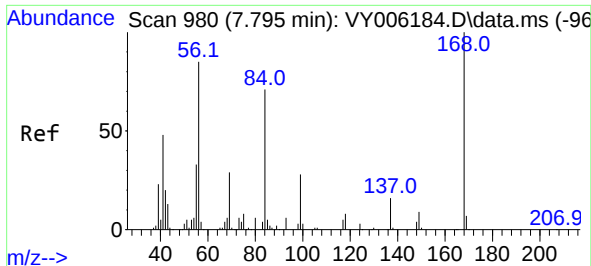

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35




Instrument :
MSVOA_Y
ClientSampleId :
SB-4(3-3.5)


Tgt Ion:168 Resp: 120245
Ion Ratio Lower Upper
168 100
99 53.9 46.9 70.3

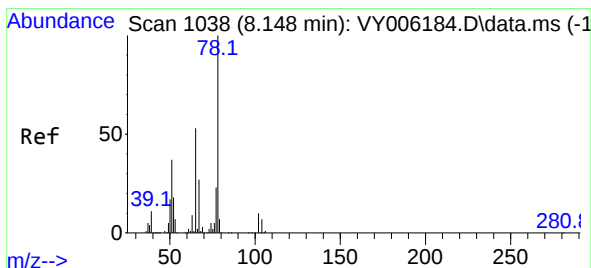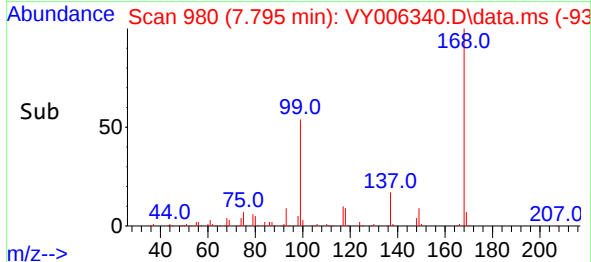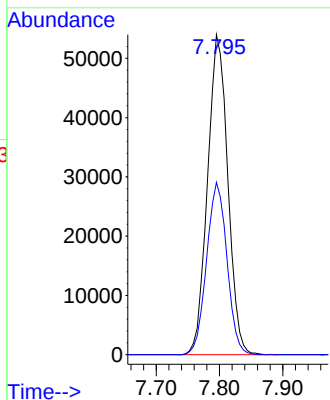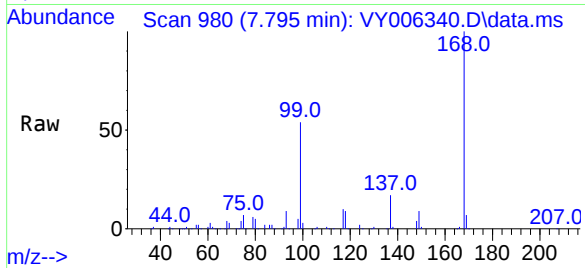

#33
1,2-Dichloroethane-d4
Concen: 61.74 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35

Tgt Ion: 65 Resp: 79457
Ion Ratio Lower Upper
65 100
67 50.0 0.0 99.4


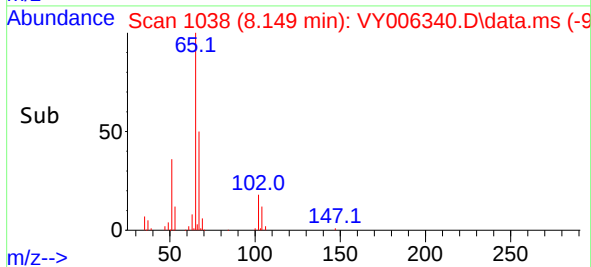
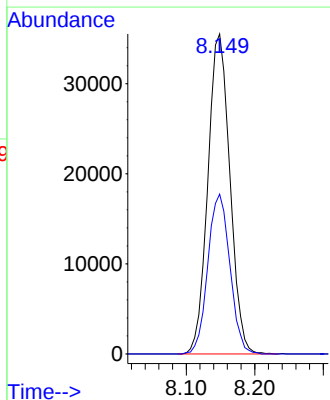
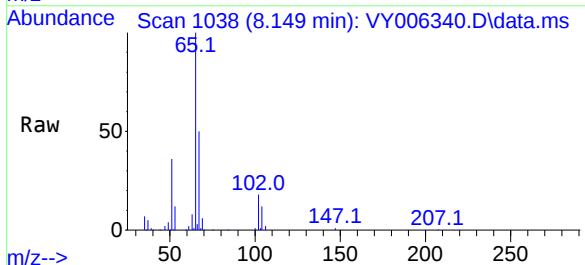


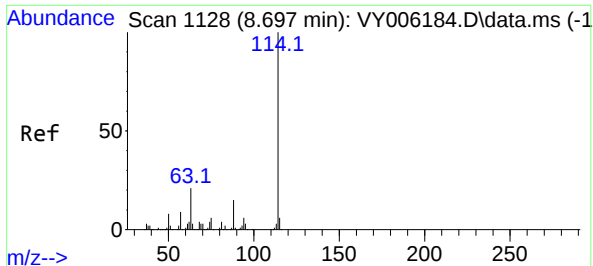

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35




Instrument :
MSVOA_Y
ClientSampleId :
SB-4(3-3.5)


Tgt Ion:	114	Resp:	197743
Ion	Ratio	Lower	Upper
114	100		
63	20.7	0.0	43.2
88	15.3	0.0	31.8

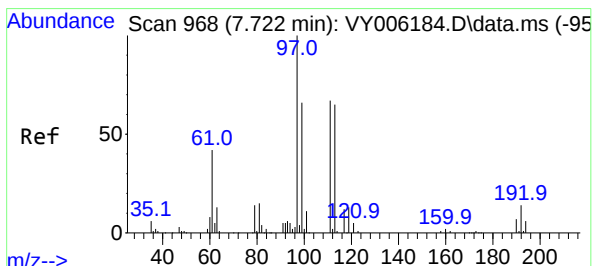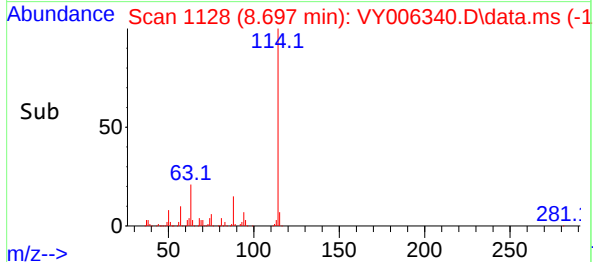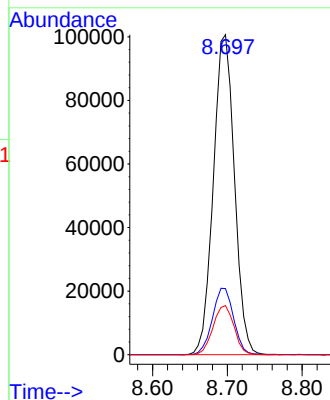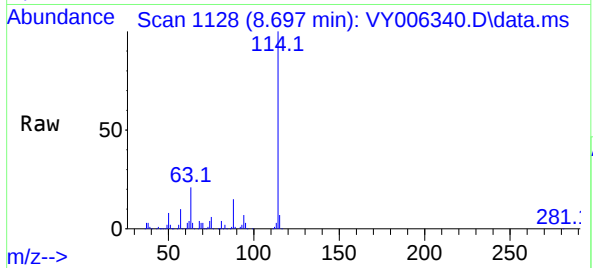

#35
Dibromofluoromethane
Concen: 56.31 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.006 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35

Tgt Ion:	113	Resp:	59491
Ion	Ratio	Lower	Upper
113	100		
111	103.3	82.6	124.0
192	23.0	17.6	26.4


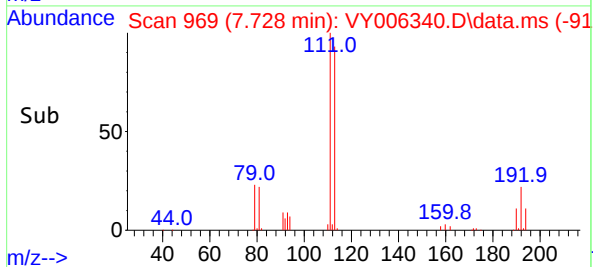
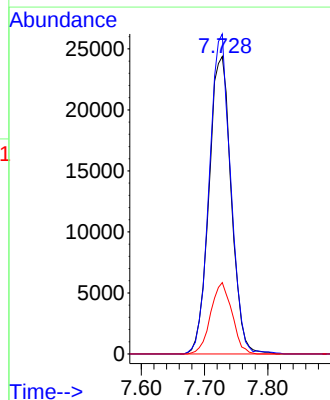
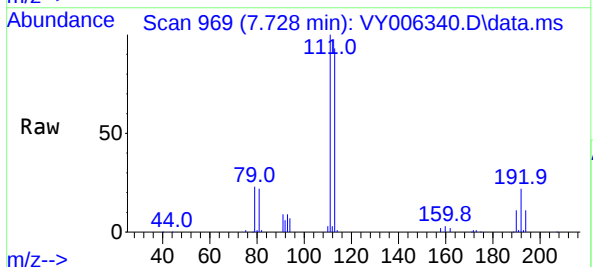


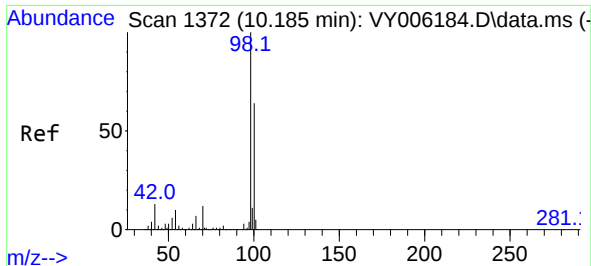

#50
Toluene-d8
Concen: 56.71 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35




Instrument :
MSVOA_Y
ClientSampleId :
SB-4(3-3.5)


Tgt Ion: 98 Resp: 250738
Ion Ratio Lower Upper
98 100
100 62.8 50.2 75.2

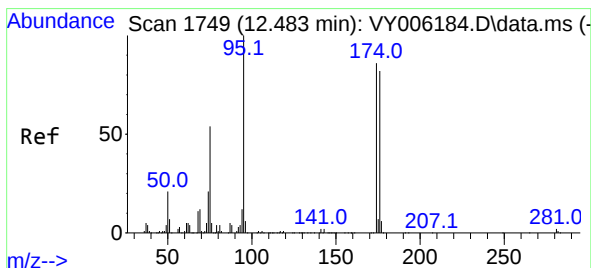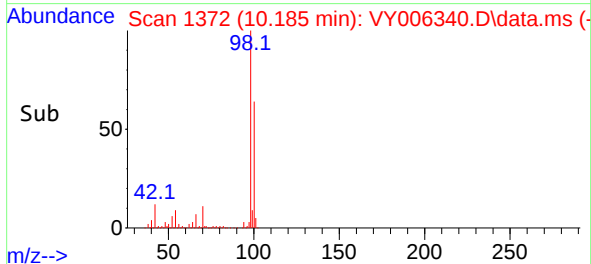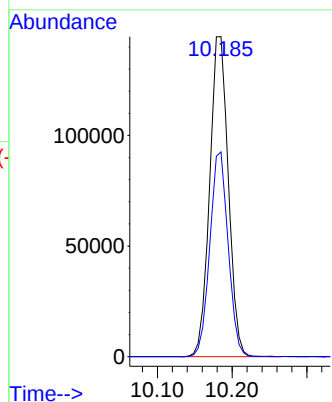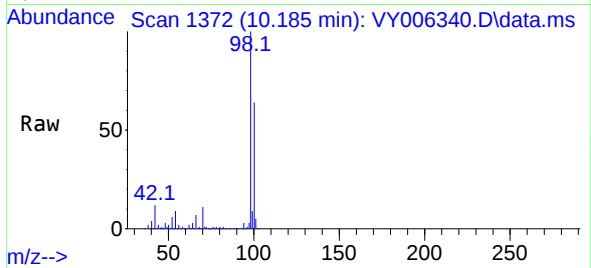

#62
4-Bromofluorobenzene
Concen: 49.64 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35

Tgt Ion: 95 Resp: 74568
Ion Ratio Lower Upper
95 100
174 95.4 0.0 177.0
176 92.1 0.0 175.8


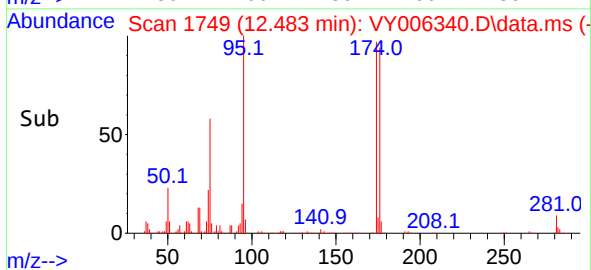
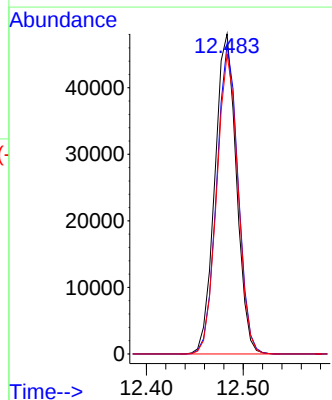
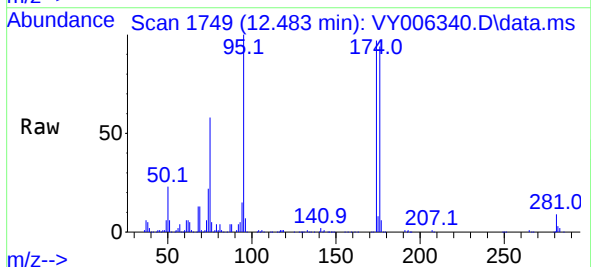


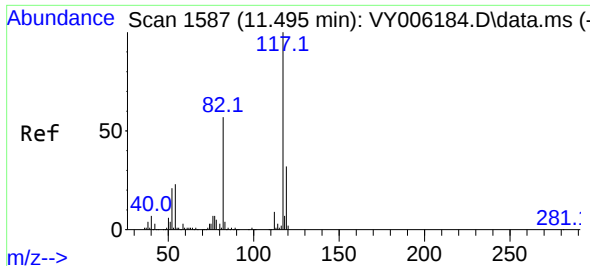

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35

Instrument :
MSVOA_Y
ClientSampleId :
SB-4(3-3.5)

Tgt Ion:	117	Resp:	183110
Ion	Ratio	Lower	Upper
117	100		
82	55.6	43.0	64.4
119	31.9	25.4	38.0

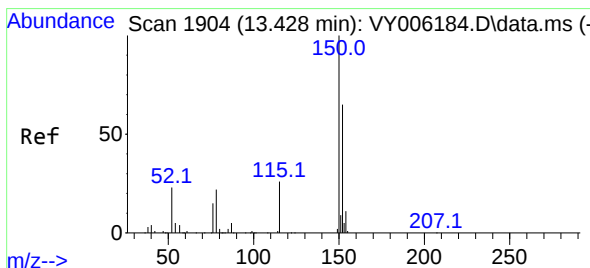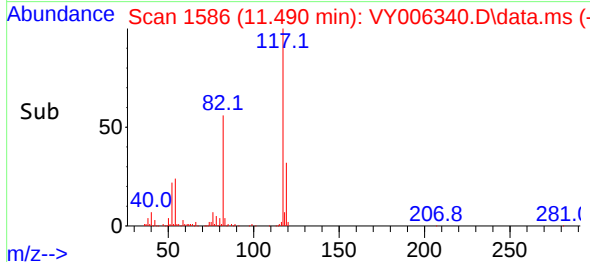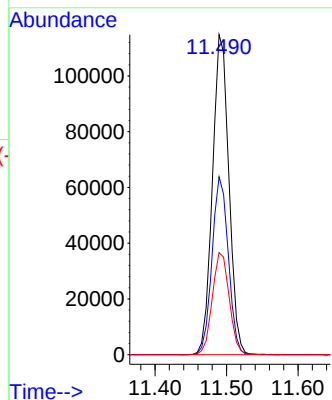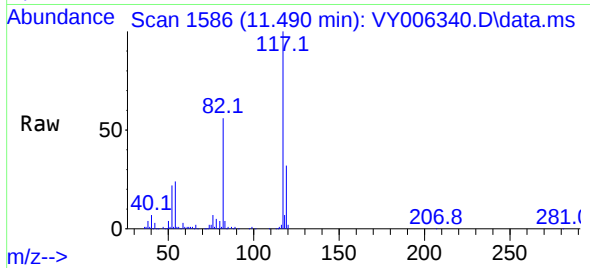

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY006340.D
Acq: 07 Oct 2021 18:35

Tgt Ion:	152	Resp:	82843
Ion	Ratio	Lower	Upper
152	100		
115	54.3	28.2	84.7
150	156.9	0.0	347.6

