

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100821\
 Data File : VY006345.D
 Acq On : 07 Oct 2021 20:31
 Operator : SY/MD
 Sample : M4117-18
 Misc : 4.36G/5ML/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-5(6.5-7.0)

Quant Time: Oct 08 07:15:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 28 17:44:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	50557	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	83069	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	80995	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	37985	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	37870	69.99	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	139.98%
35) Dibromofluoromethane	7.722	113	26863	60.53	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	121.06%
50) Toluene-d8	10.185	98	107657	57.96	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	115.92%
62) 4-Bromofluorobenzene	12.483	95	32851	52.06	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	104.12%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100821\
Data File : VY006345.D
Acq On : 07 Oct 2021 20:31
Operator : SY/MD
Sample : M4117-18
Misc : 4.36G/5ML/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-5(6.5-7.0)

Quant Time: Oct 08 07:15:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 17:44:36 2021
Response via : Initial Calibration




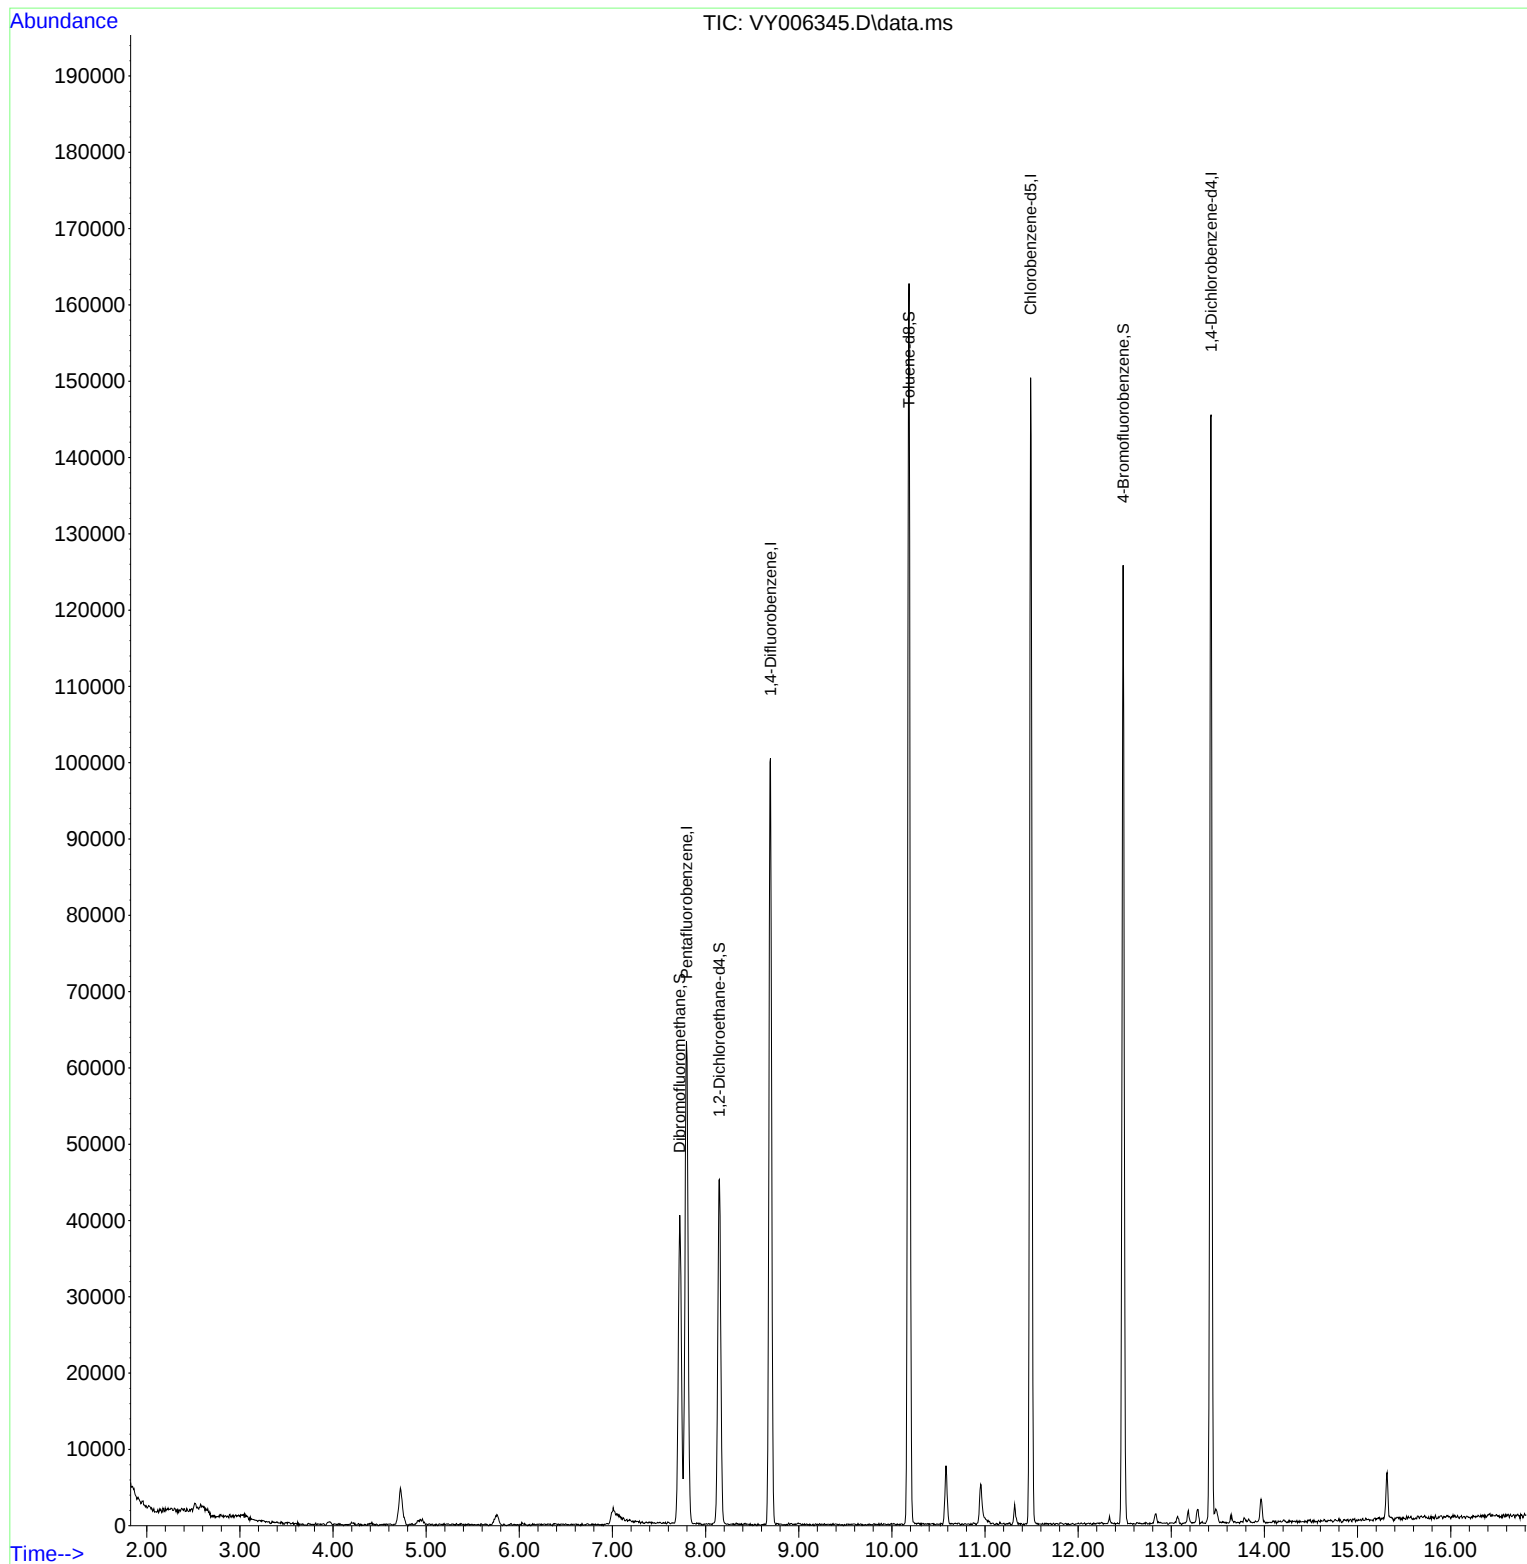


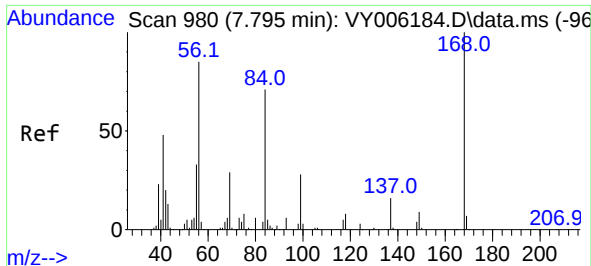

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31




Instrument :
MSVOA_Y
ClientSampleId :
SB-5(6.5-7.0)


Tgt Ion:168 Resp: 50557
Ion Ratio Lower Upper
168 100
99 52.8 46.9 70.3

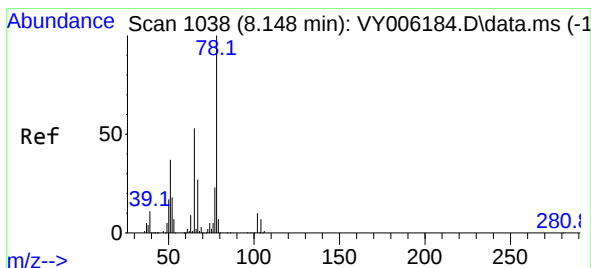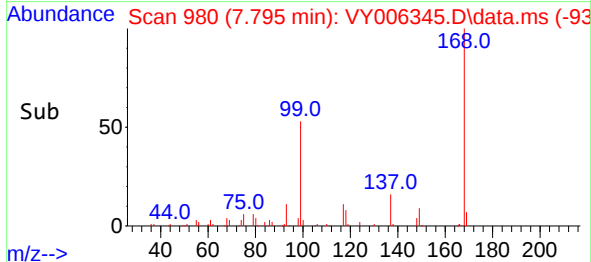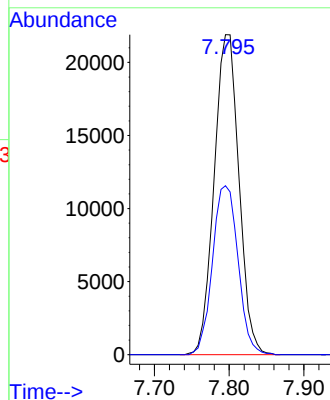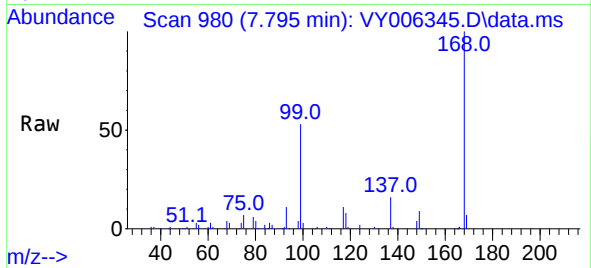

#33
1,2-Dichloroethane-d4
Concen: 69.99 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31

Tgt Ion: 65 Resp: 37870
Ion Ratio Lower Upper
65 100
67 50.1 0.0 99.4


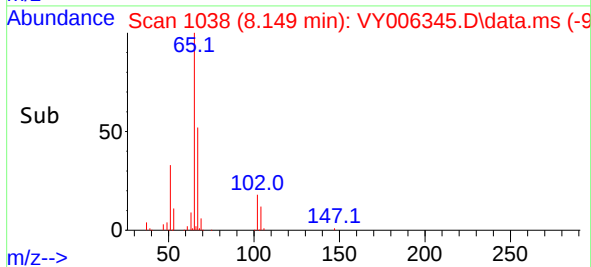
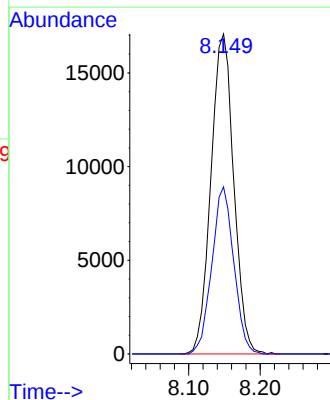
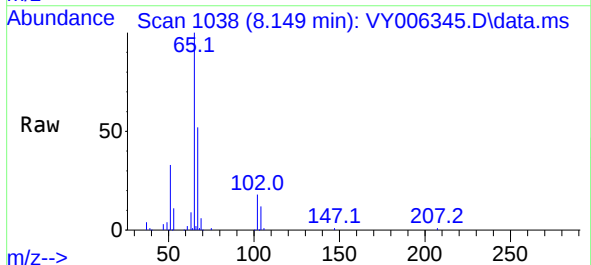


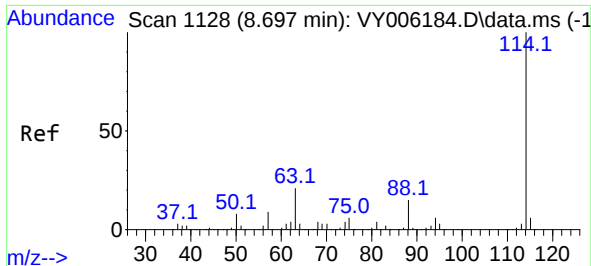

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31




Instrument :
MSVOA_Y
ClientSampleId :
SB-5(6.5-7.0)


Tgt Ion:	114	Resp:	83069
Ion	Ratio	Lower	Upper
114	100		
63	21.1	0.0	43.2
88	15.1	0.0	31.8

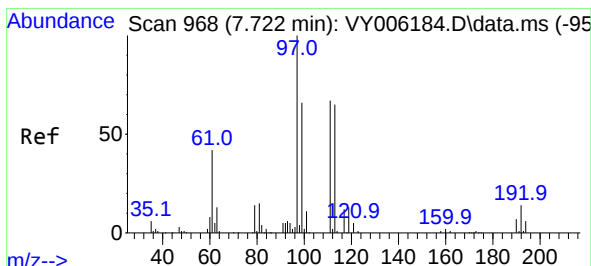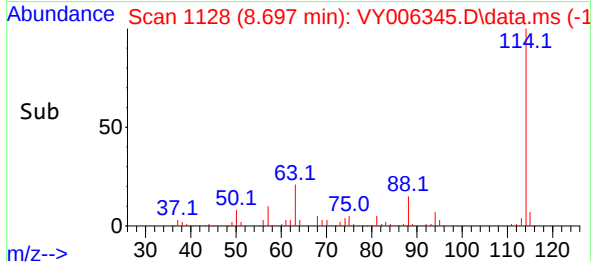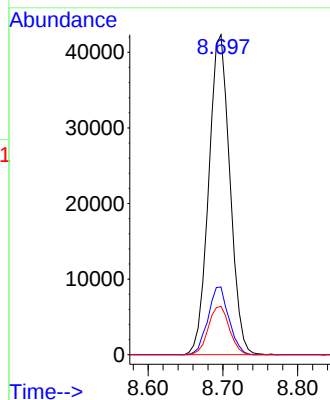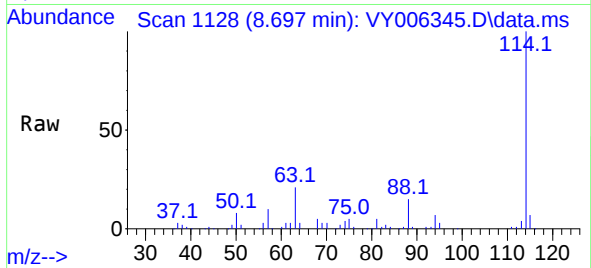

#35
Dibromofluoromethane
Concen: 60.53 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31

Tgt Ion:	113	Resp:	26863
Ion	Ratio	Lower	Upper
113	100		
111	103.4	82.6	124.0
192	23.0	17.6	26.4


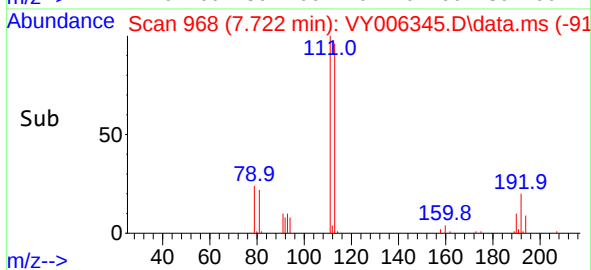
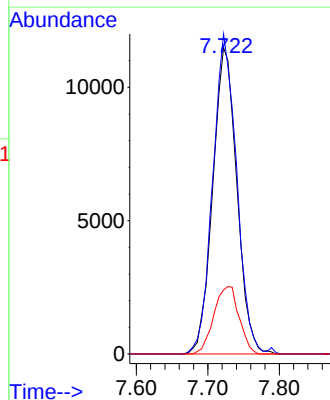
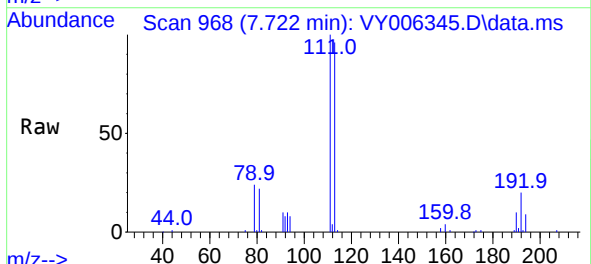


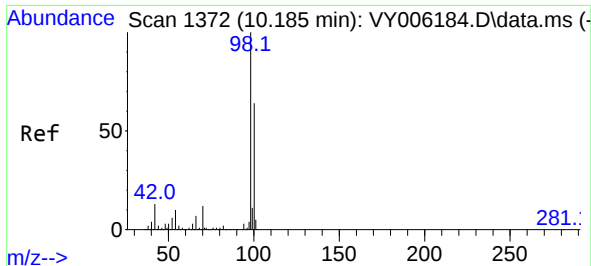

#50
Toluene-d8
Concen: 57.96 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31




Instrument :
MSVOA_Y
ClientSampleId :
SB-5(6.5-7.0)


Tgt Ion: 98 Resp: 107657
Ion Ratio Lower Upper
98 100
100 62.3 50.2 75.2

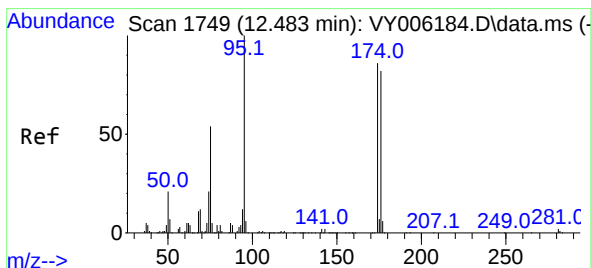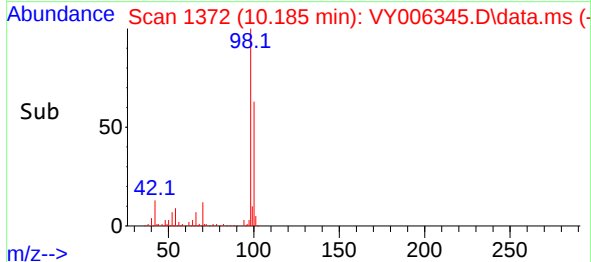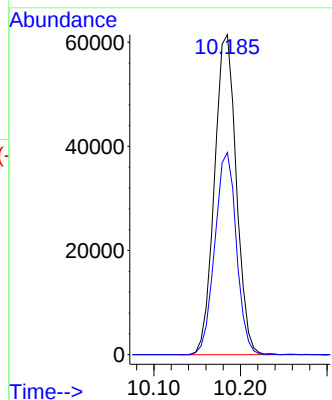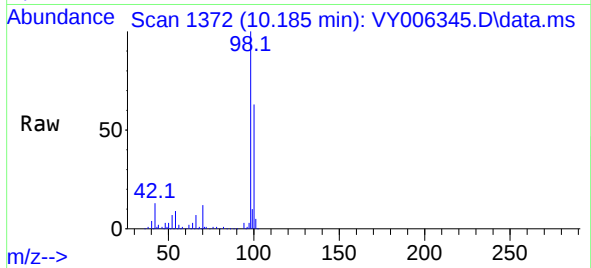

#62
4-Bromofluorobenzene
Concen: 52.06 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31

Tgt Ion: 95 Resp: 32851
Ion Ratio Lower Upper
95 100
174 96.2 0.0 177.0
176 89.7 0.0 175.8


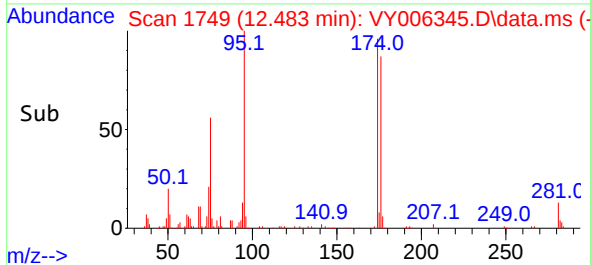
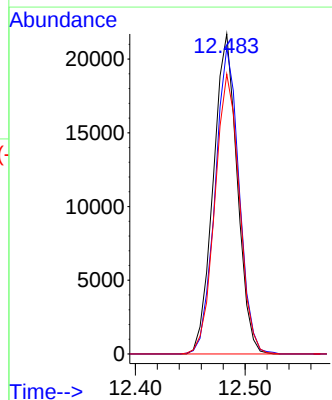
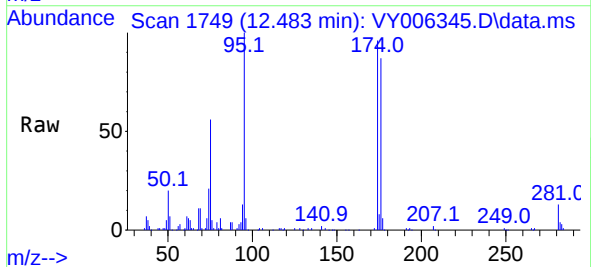


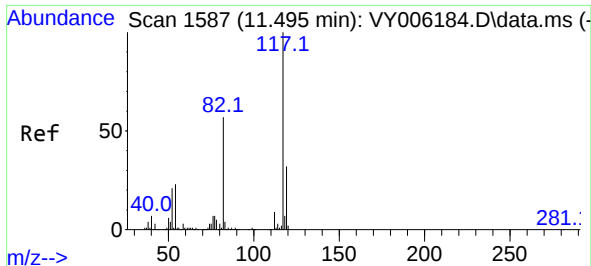

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31

Instrument :
MSVOA_Y
ClientSampleId :
SB-5(6.5-7.0)

Tgt Ion:	117	Resp:	80995
Ion	Ratio	Lower	Upper
117	100		
82	55.3	43.0	64.4
119	31.4	25.4	38.0

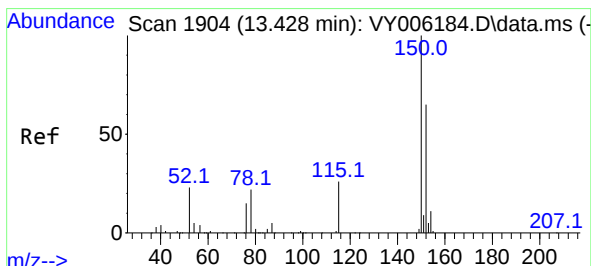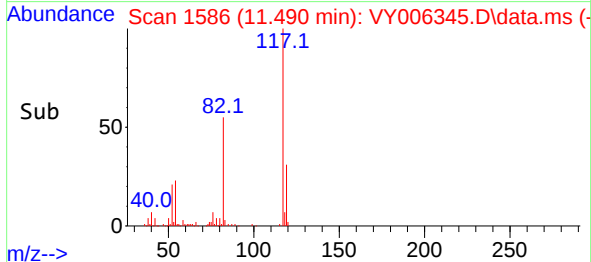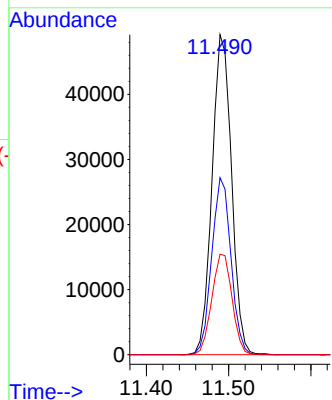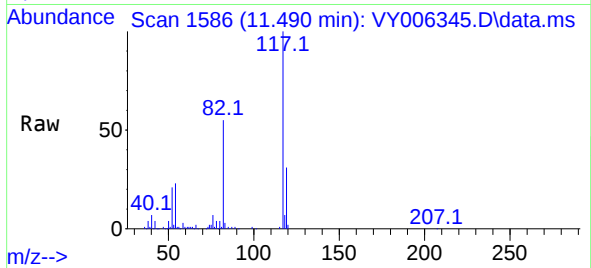

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY006345.D
Acq: 07 Oct 2021 20:31

Tgt Ion:	152	Resp:	37985
Ion	Ratio	Lower	Upper
152	100		
115	54.6	28.2	84.7
150	153.9	0.0	347.6

