


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY101019\
Data File : VY000249.D
Acq On : 10 Oct 2019 11:10
Operator : SY/MD
Sample : BFB
Misc : 5.0ml/MSVOA Y/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y100819W.M
Title : SW846 8260
Last Update : Fri Oct 11 07:25:41 2019

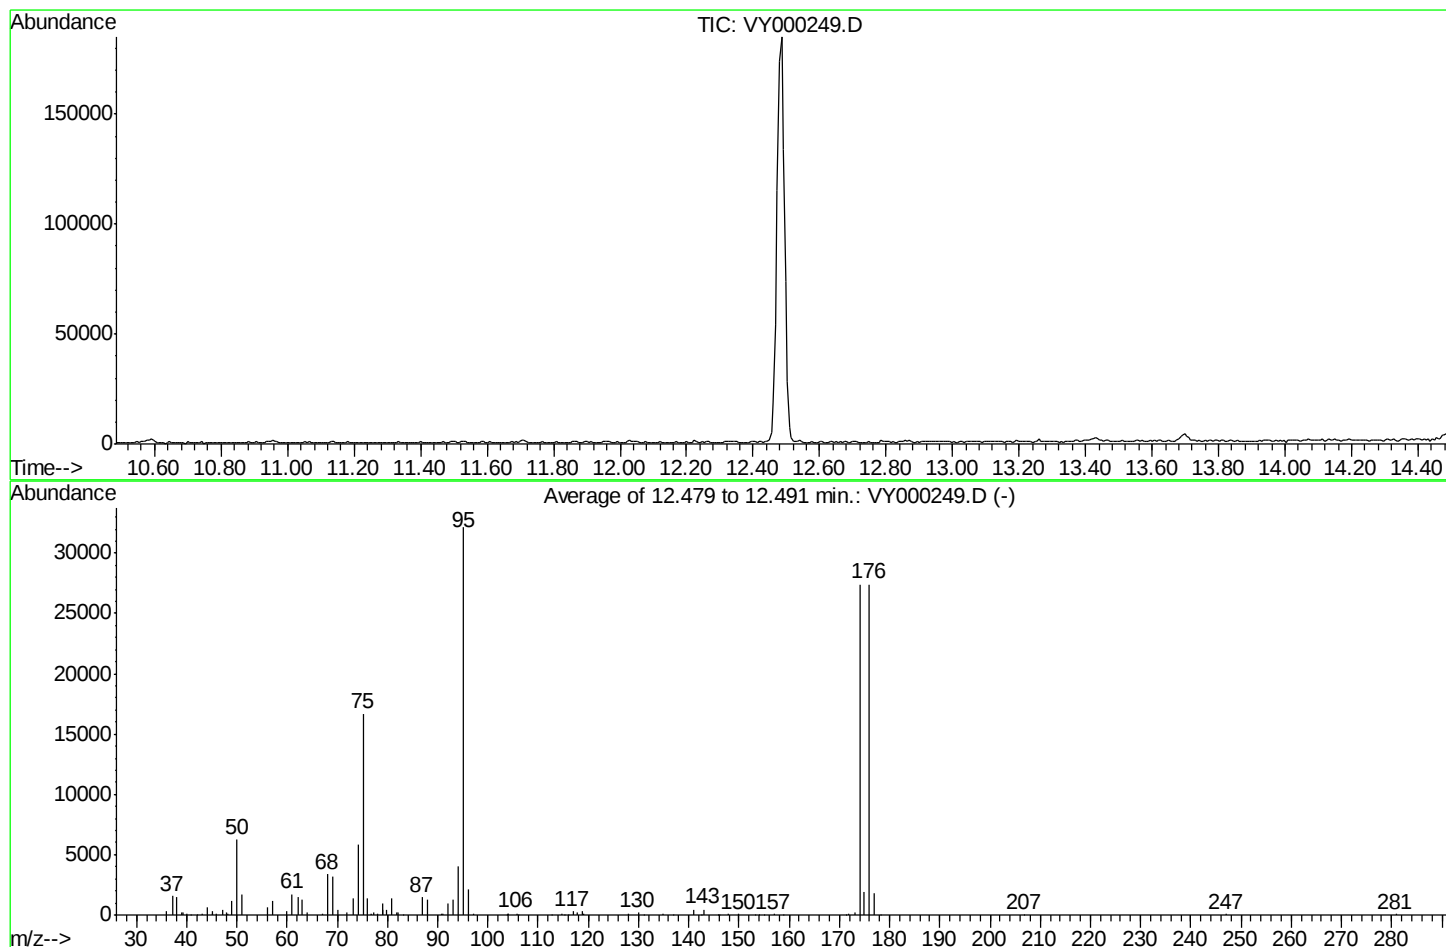

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6225	PASS
75	95	30	60	52.0	16708	PASS
95	95	100	100	100.0	32141	PASS
96	95	5	9	6.7	2147	PASS
173	174	0.00	2	0.8	228	PASS
174	95	50	100	85.1	27338	PASS
175	174	5	9	7.0	1910	PASS
176	174	95	101	100.3	27426	PASS
177	176	5	9	6.5	1770	PASS