
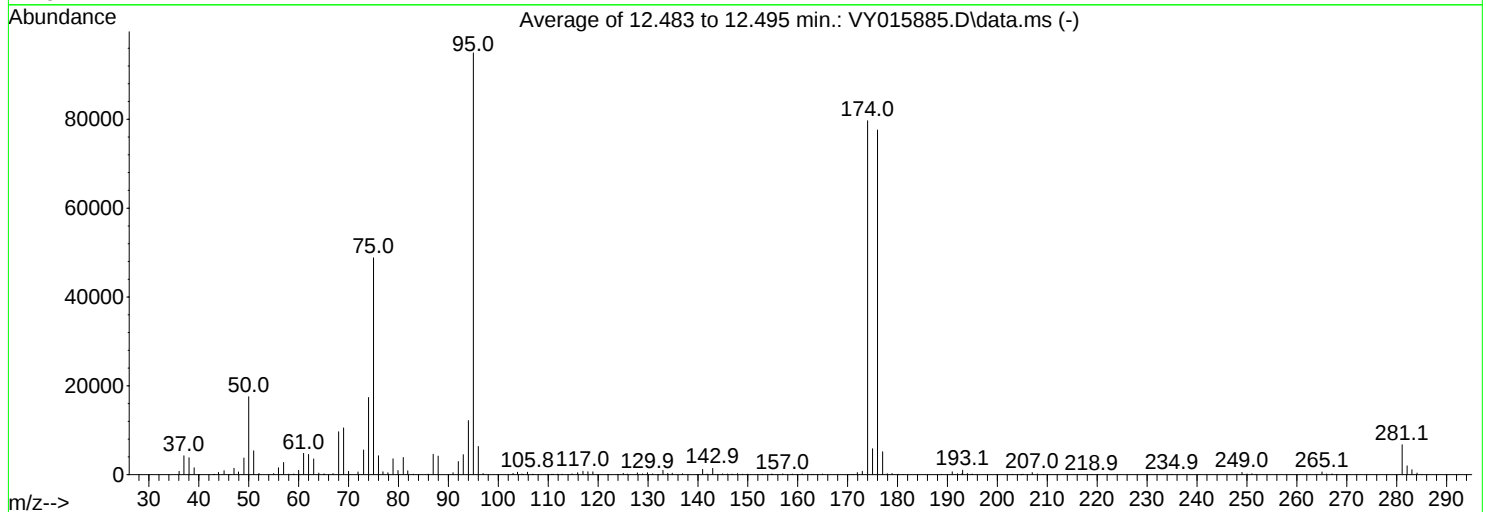


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101023\
Data File : VY015885.D
Acq On : 10 Oct 2023 09:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100923S.M
Title : SW846 8260
Last Update : Tue Oct 10 07:06:18 2023

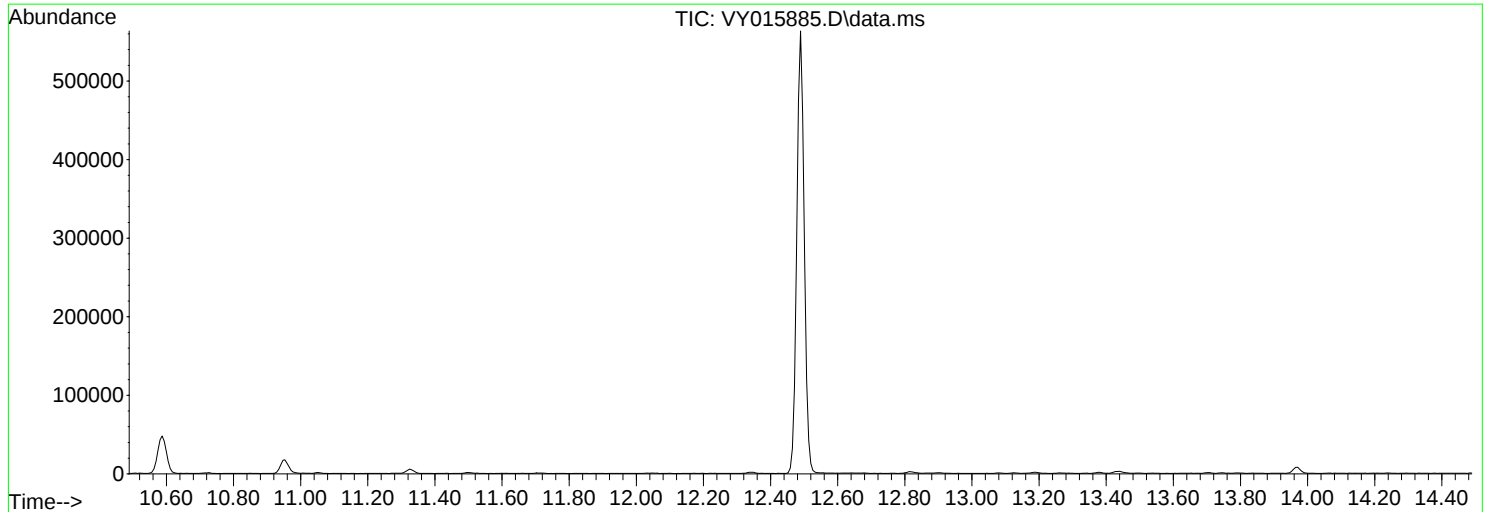

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	17561	PASS
75	95	30	60	51.4	48835	PASS
95	95	100	100	100.0	94968	PASS
96	95	5	9	6.7	6351	PASS
173	174	0.00	2	0.9	743	PASS
174	95	50	100	83.9	79672	PASS
175	174	5	9	7.3	5846	PASS
176	174	95	101	97.4	77595	PASS
177	176	5	9	6.6	5139	PASS