
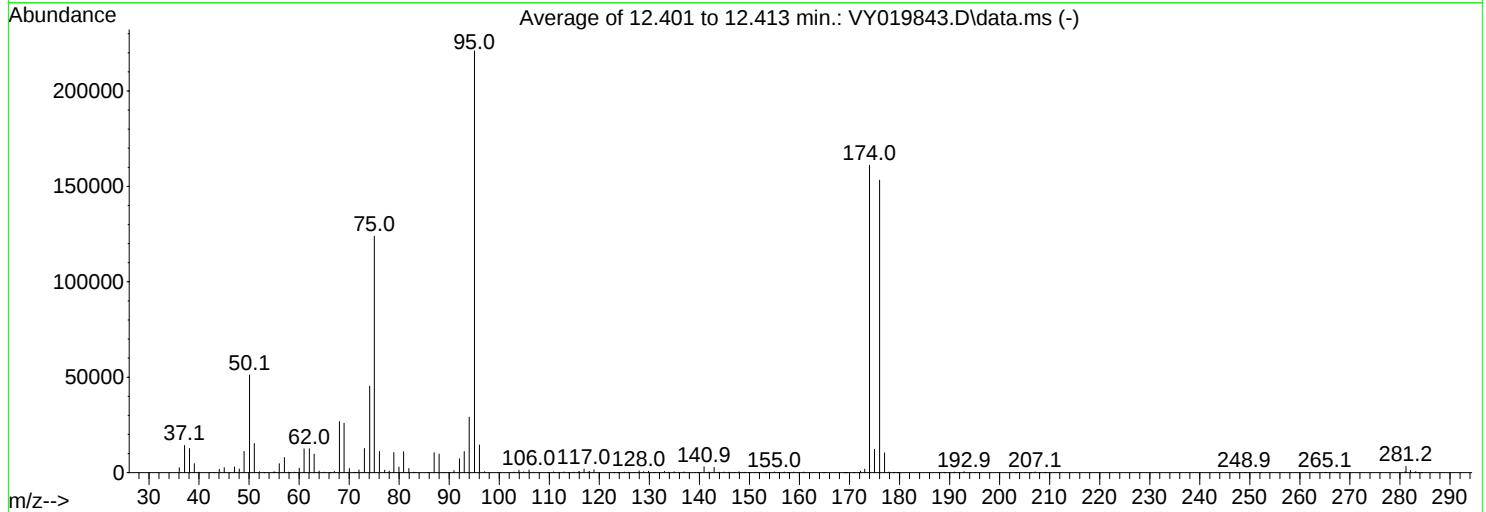


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101024\
Data File : VY019843.D
Acq On : 10 Oct 2024 08:53
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Thu Oct 10 05:30:07 2024

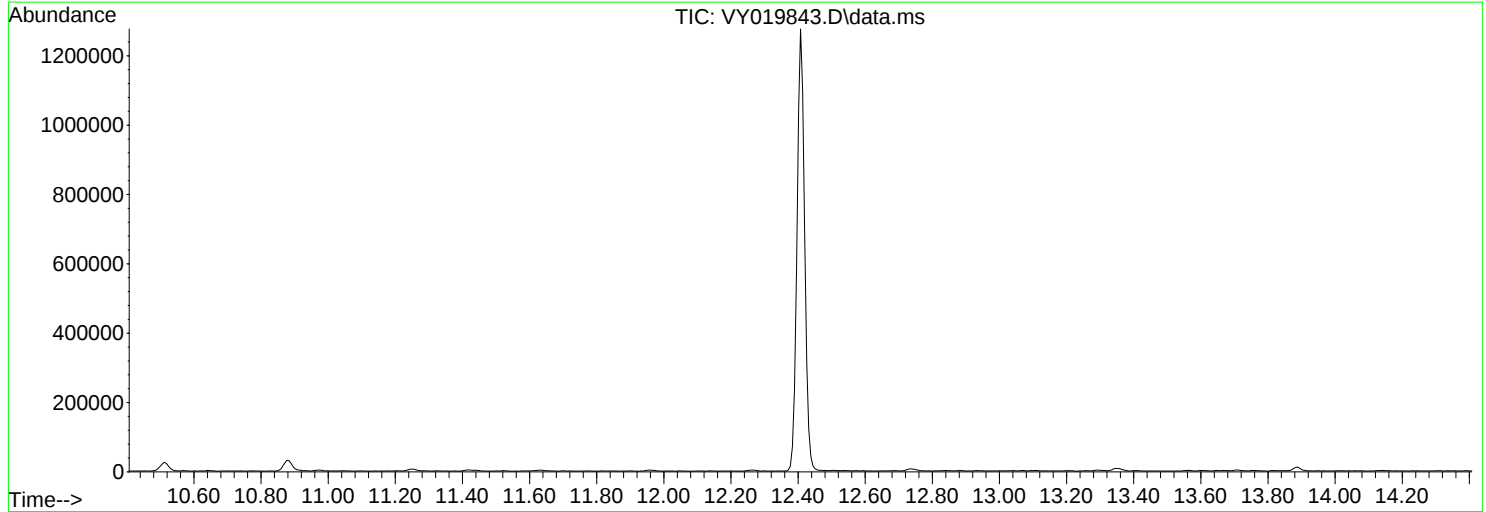

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	51269	PASS
75	95	30	60	56.1	123899	PASS
95	95	100	100	100.0	221035	PASS
96	95	5	9	6.6	14550	PASS
173	174	0.00	2	1.1	1812	PASS
174	95	50	100	72.9	161109	PASS
175	174	5	9	7.6	12236	PASS
176	174	95	101	95.1	153280	PASS
177	176	5	9	6.8	10373	PASS