
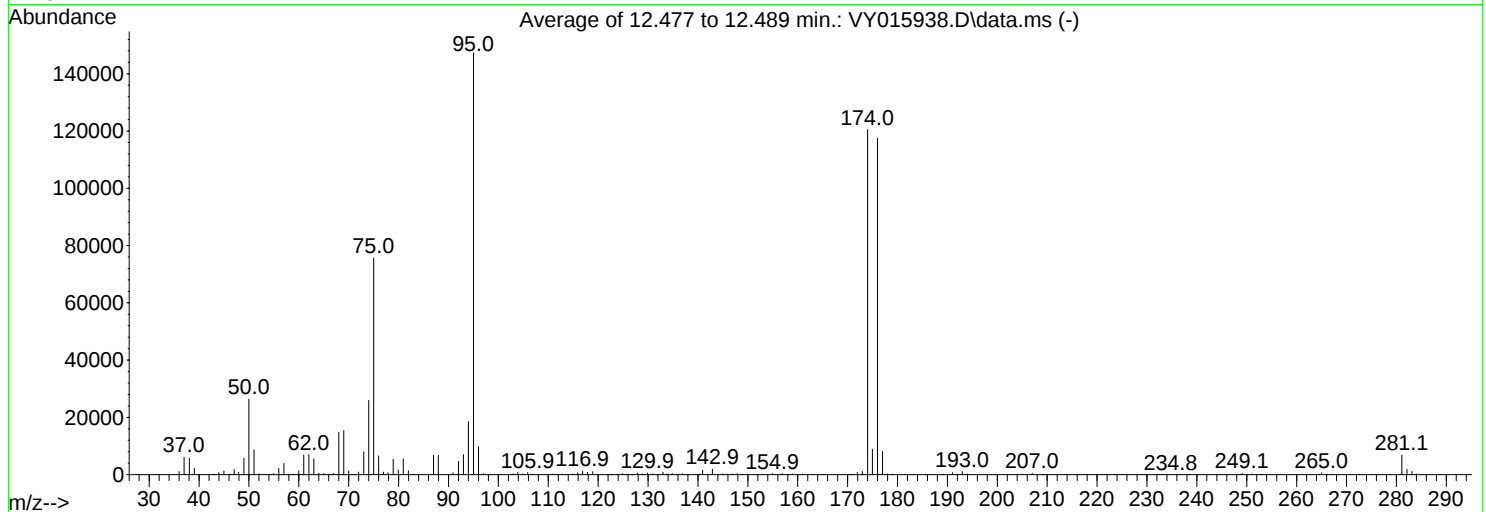


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101223\
Data File : VY015938.D
Acq On : 12 Oct 2023 16:48
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101223S.M
Title : SW846 8260
Last Update : Fri Oct 13 13:13:02 2023

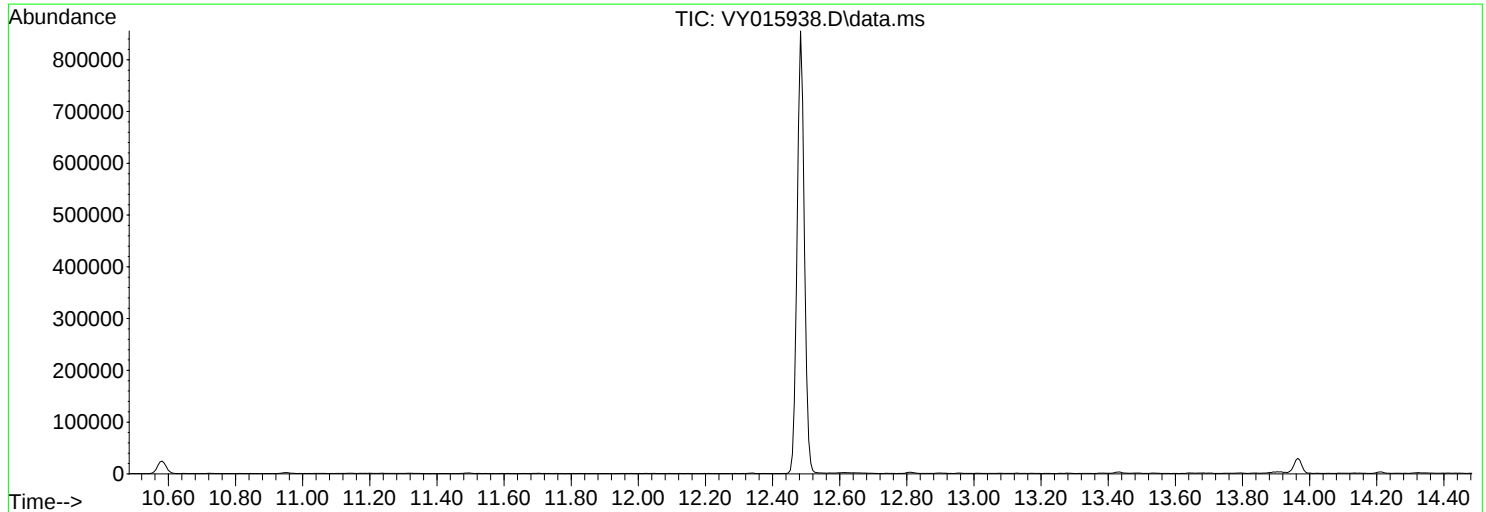

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	26397	PASS
75	95	30	60	51.4	75672	PASS
95	95	100	100	100.0	147307	PASS
96	95	5	9	6.7	9806	PASS
173	174	0.00	2	0.9	1109	PASS
174	95	50	100	81.8	120488	PASS
175	174	5	9	7.4	8872	PASS
176	174	95	101	97.5	117445	PASS
177	176	5	9	6.9	8050	PASS