
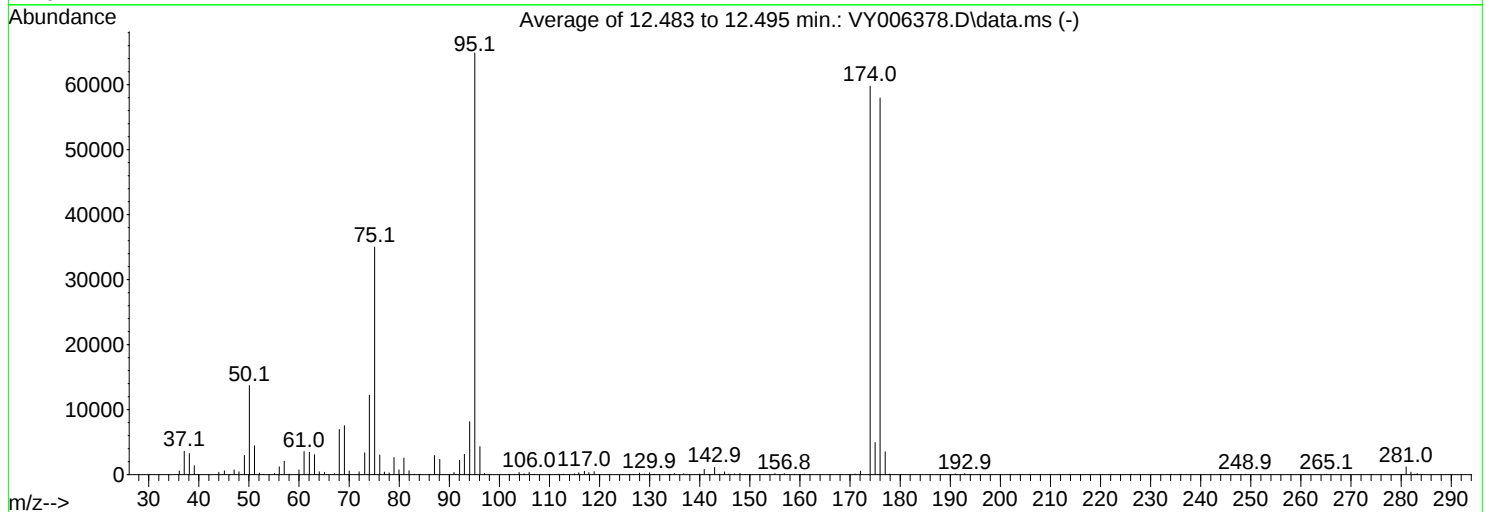


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101321\
 Data File : VY006378.D
 Acq On : 13 Oct 2021 09:14
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
 Title : SW846 8260
 Last Update : Tue Sep 28 17:44:36 2021

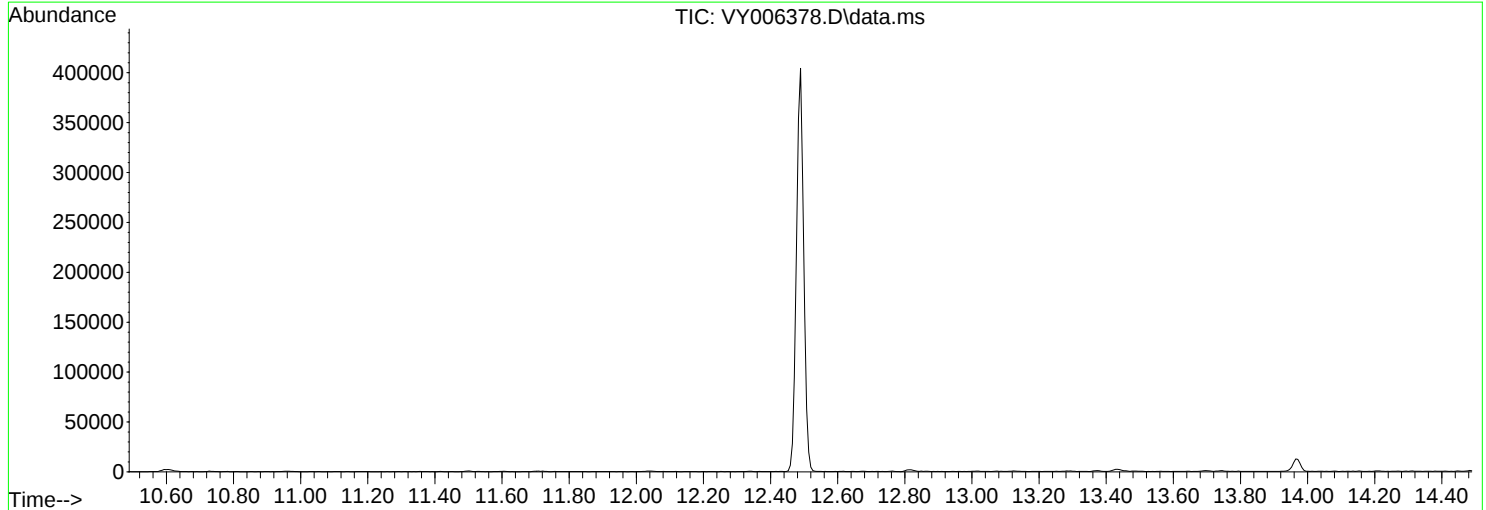

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	13715	PASS
75	95	30	60	53.9	35008	PASS
95	95	100	100	100.0	64901	PASS
96	95	5	9	6.6	4311	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.1	59781	PASS
175	174	5	9	8.3	4943	PASS
176	174	95	101	97.0	57960	PASS
177	176	5	9	6.1	3523	PASS