
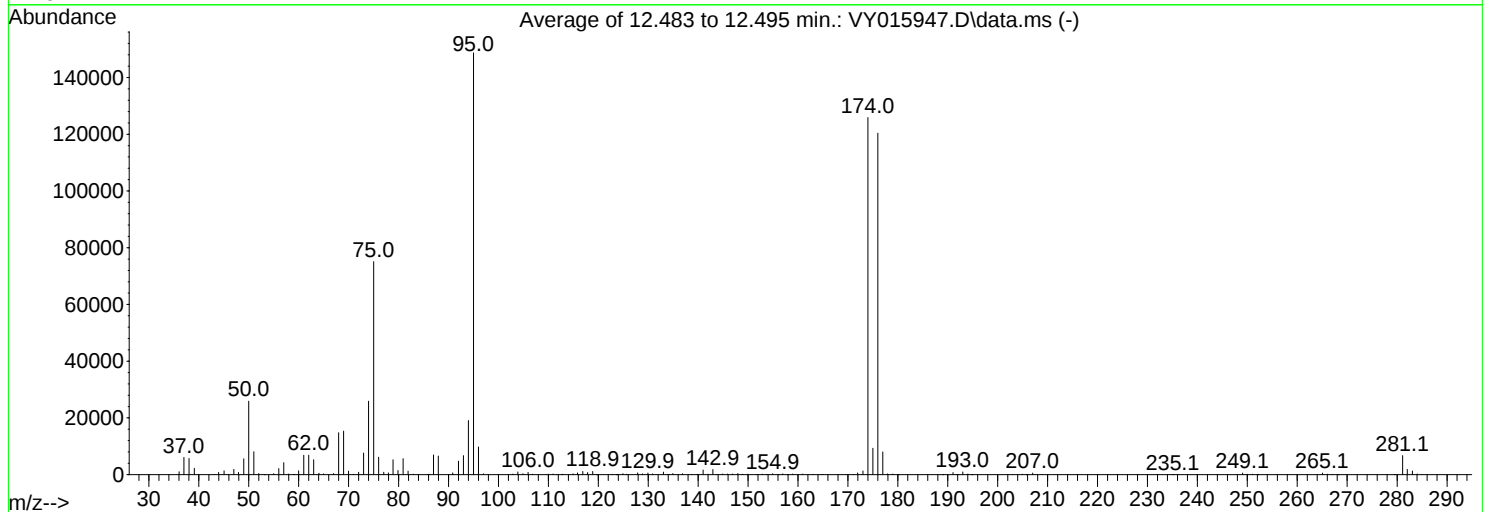


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101323\
Data File : VY015947.D
Acq On : 13 Oct 2023 09:04
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101223S.M
Title : SW846 8260
Last Update : Fri Oct 13 13:13:02 2023

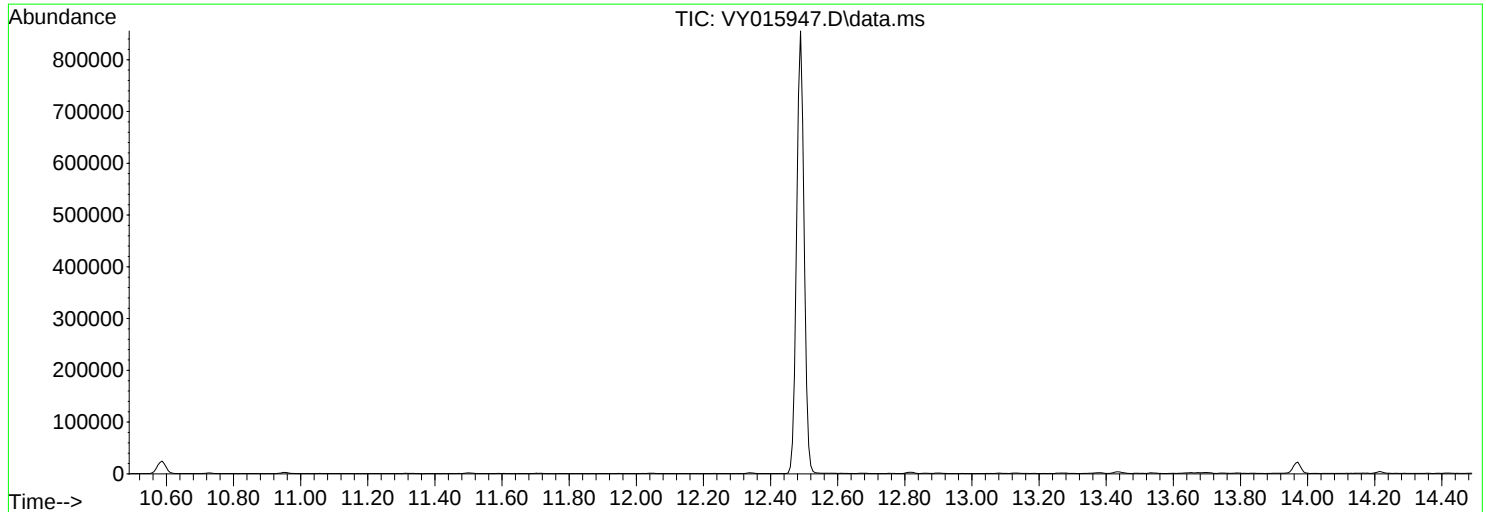

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	25896	PASS
75	95	30	60	50.5	75075	PASS
95	95	100	100	100.0	148704	PASS
96	95	5	9	6.6	9775	PASS
173	174	0.00	2	1.0	1291	PASS
174	95	50	100	84.7	125920	PASS
175	174	5	9	7.4	9313	PASS
176	174	95	101	95.6	120397	PASS
177	176	5	9	6.7	8019	PASS