


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv101519\
 Data File : VY000310.D
 Acq On : 15 Oct 2019 10:12
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
 Title : SW846 8260
 Last Update : Mon Oct 14 08:10:23 2019

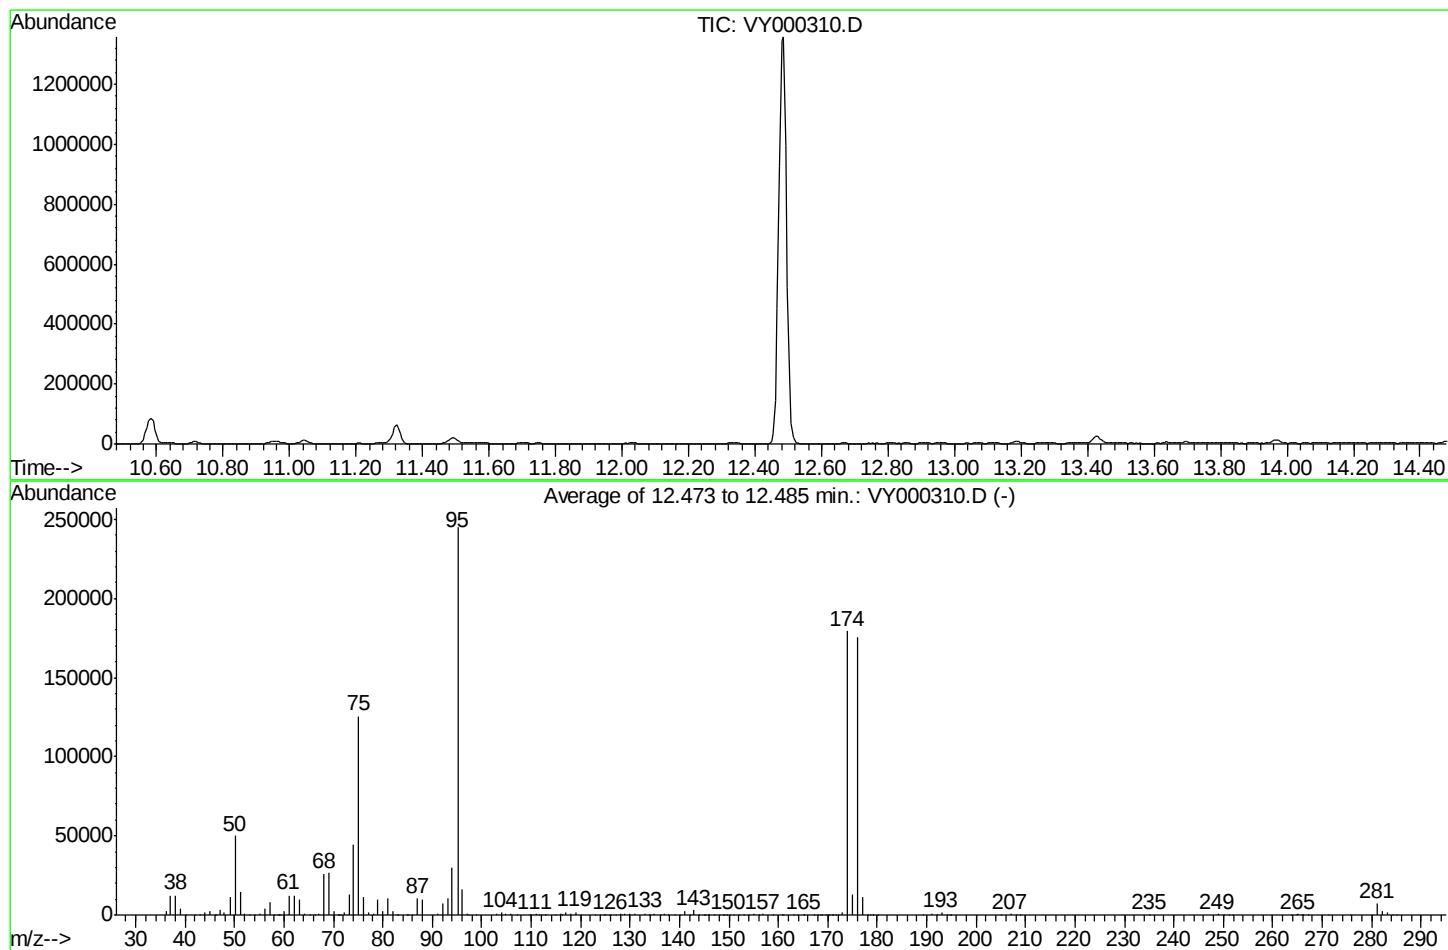

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	49821	PASS
75	95	30	60	51.2	125397	PASS
95	95	100	100	100.0	244928	PASS
96	95	5	9	6.6	16109	PASS
173	174	0.00	2	0.8	1368	PASS
174	95	50	100	73.3	179485	PASS
175	174	5	9	7.3	13129	PASS
176	174	95	101	97.6	175114	PASS
177	176	5	9	6.7	11735	PASS