
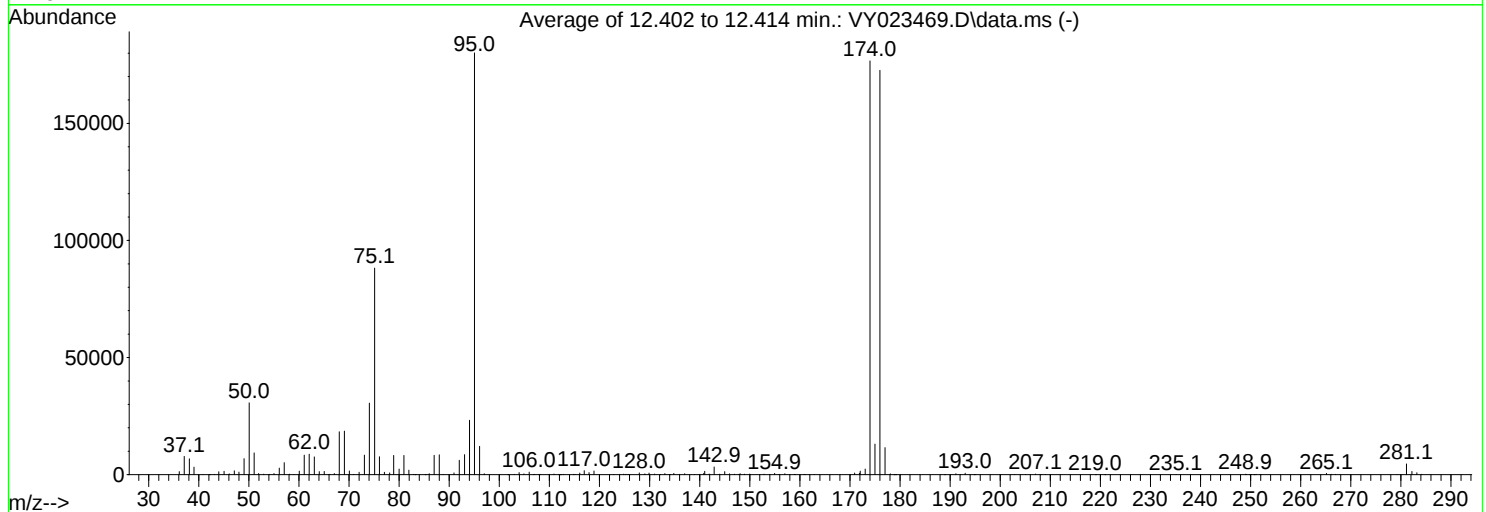


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101525\
Data File : VY023469.D
Acq On : 15 Oct 2025 10:08
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

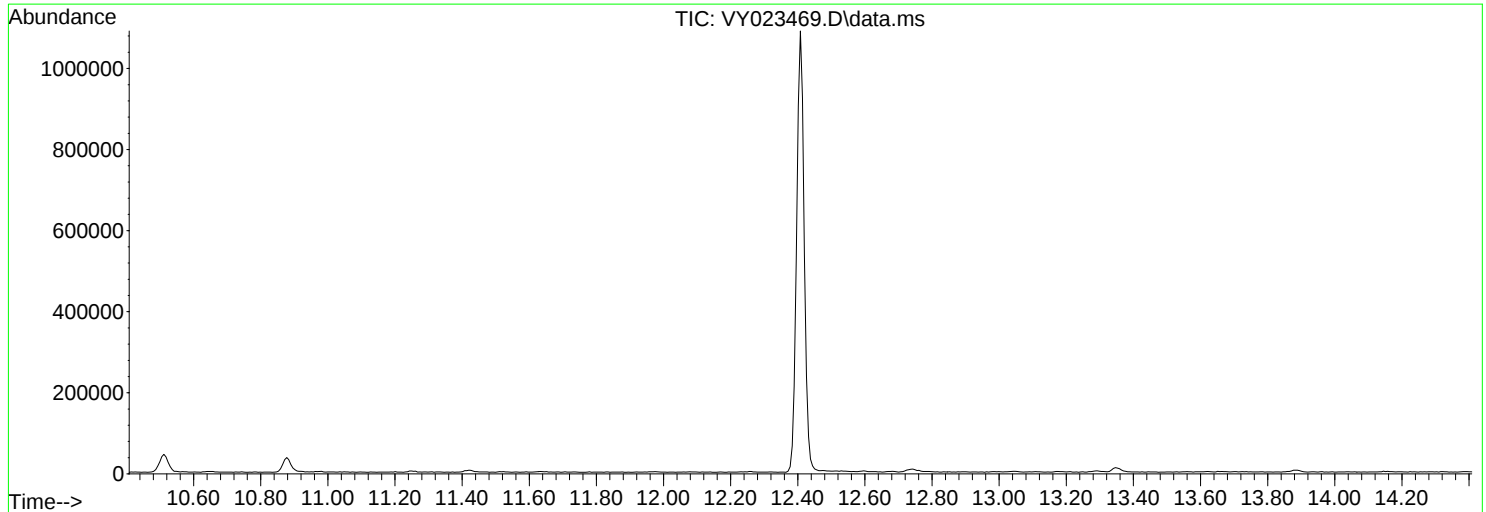

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	30659	PASS
75	95	30	60	49.0	88237	PASS
95	95	100	100	100.0	180117	PASS
96	95	5	9	6.7	12064	PASS
173	174	0.00	2	1.3	2365	PASS
174	95	50	100	98.1	176661	PASS
175	174	5	9	7.4	13058	PASS
176	174	95	101	97.7	172651	PASS
177	176	5	9	6.7	11536	PASS