
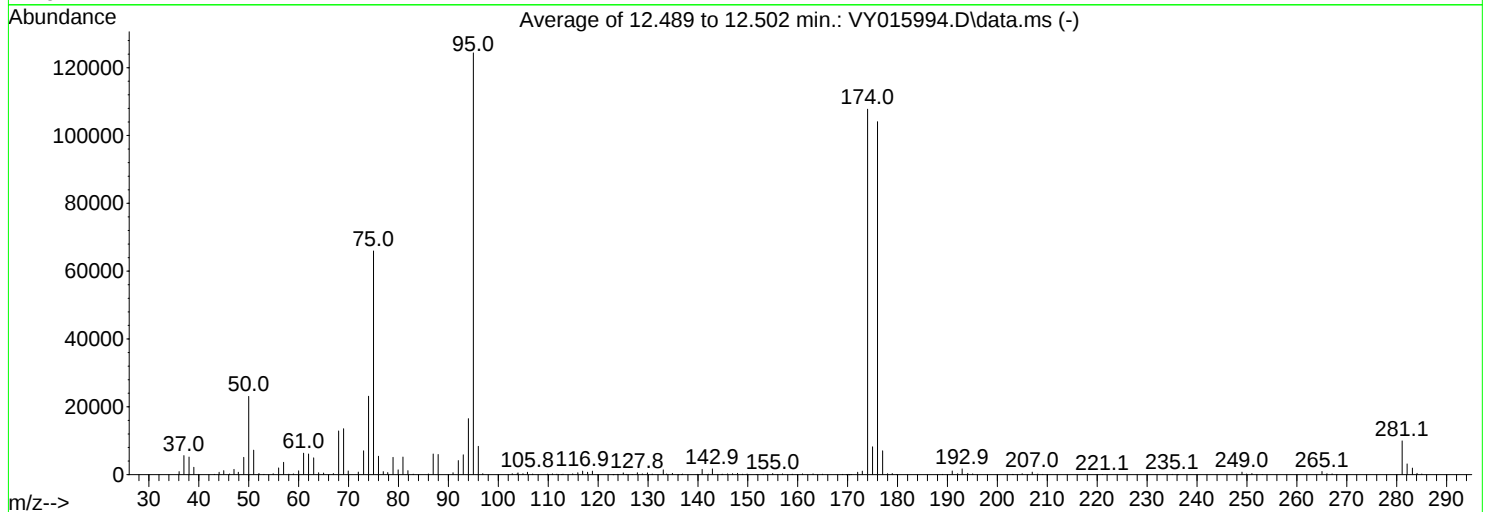


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101723\
Data File : VY015994.D
Acq On : 17 Oct 2023 08:50
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101223S.M
Title : SW846 8260
Last Update : Fri Oct 13 13:13:02 2023

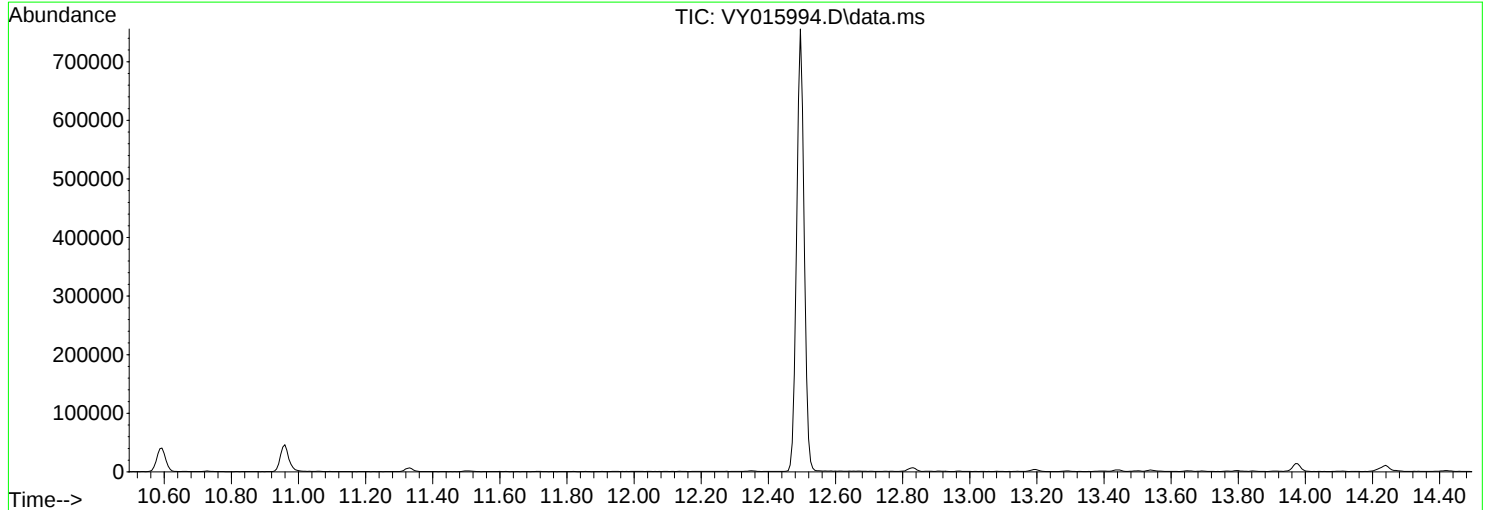

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	23091	PASS
75	95	30	60	53.0	65979	PASS
95	95	100	100	100.0	124376	PASS
96	95	5	9	6.7	8341	PASS
173	174	0.00	2	1.0	1057	PASS
174	95	50	100	86.6	107763	PASS
175	174	5	9	7.6	8206	PASS
176	174	95	101	96.6	104096	PASS
177	176	5	9	6.7	7019	PASS