


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101822\
Data File : VY010982.D
Acq On : 18 Oct 2022 09:08
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Title : SW846 8260
Last Update : Tue Oct 18 01:42:42 2022

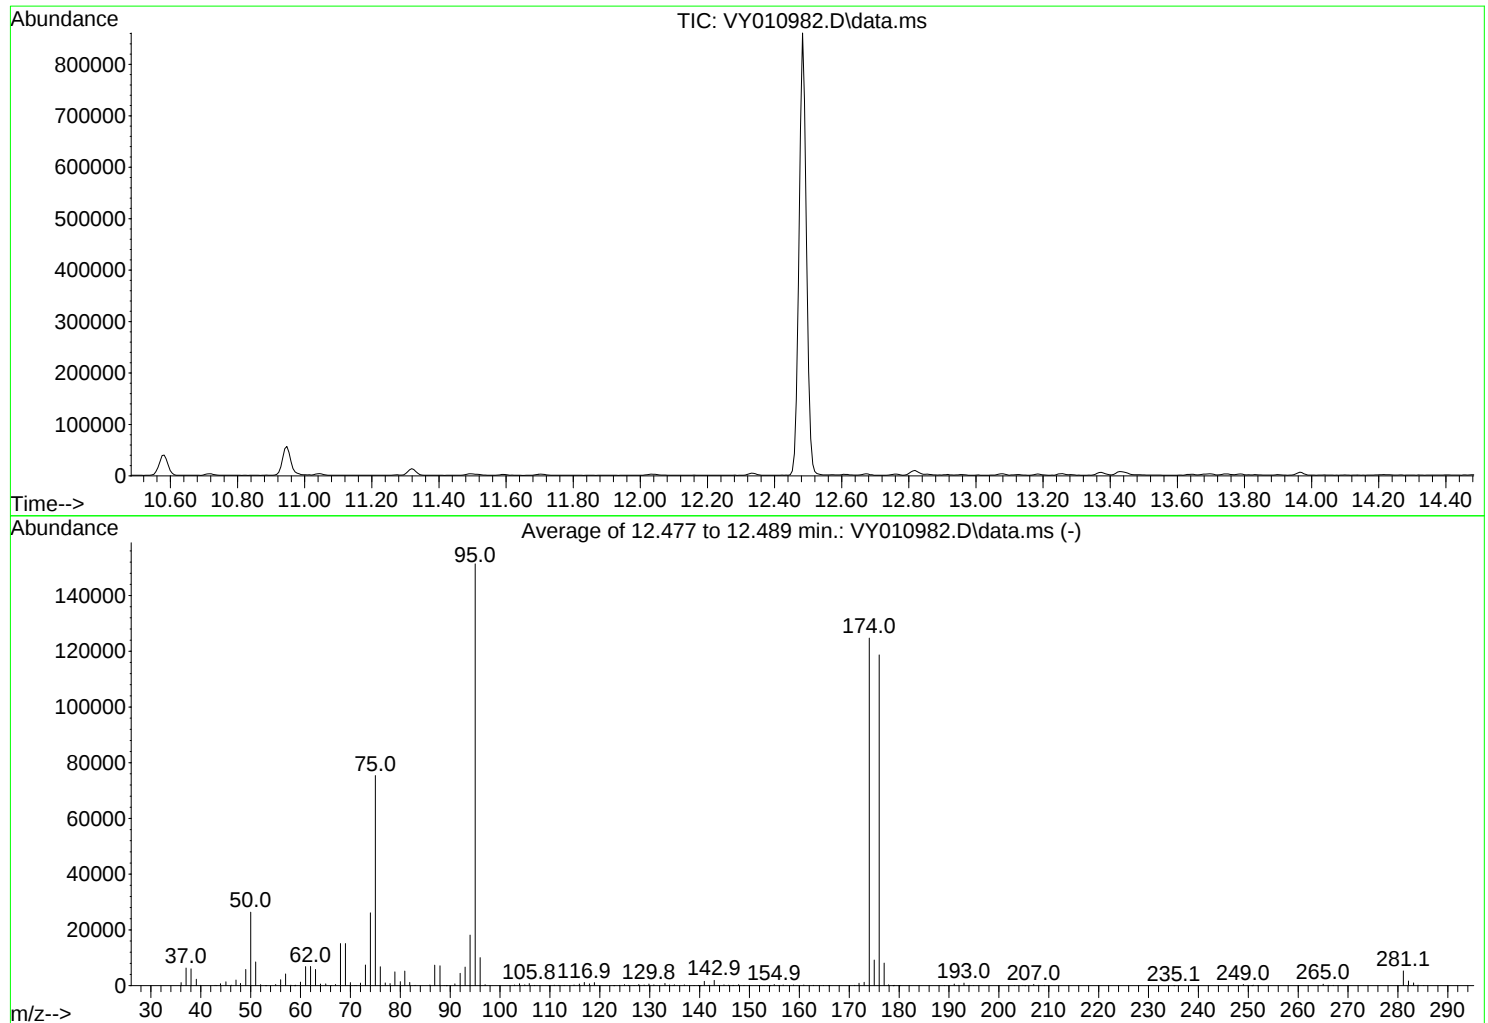

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	26384	PASS
75	95	30	60	49.8	75403	PASS
95	95	100	100	100.0	151381	PASS
96	95	5	9	6.6	10029	PASS
173	174	0.00	2	1.0	1200	PASS
174	95	50	100	82.4	124696	PASS
175	174	5	9	7.4	9203	PASS
176	174	95	101	95.2	118701	PASS
177	176	5	9	6.8	8093	PASS