
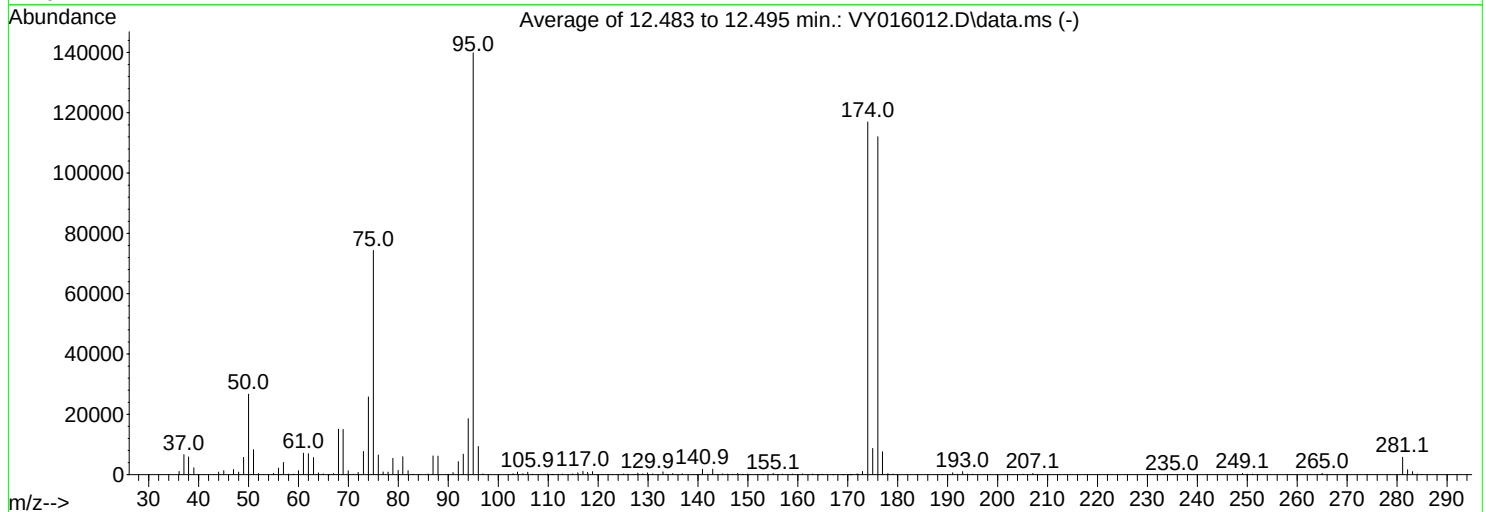


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101823\
 Data File : VY016012.D
 Acq On : 18 Oct 2023 08:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101223S.M
 Title : SW846 8260
 Last Update : Fri Oct 13 13:13:02 2023

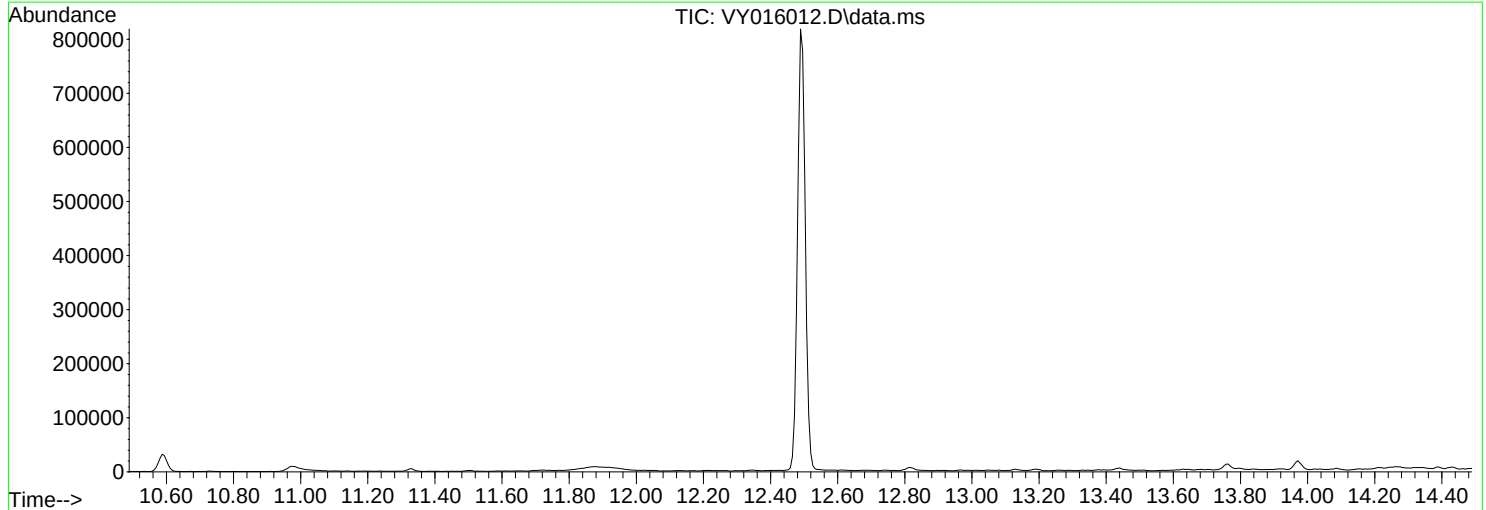

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	26699	PASS
75	95	30	60	53.1	74328	PASS
95	95	100	100	100.0	139877	PASS
96	95	5	9	6.7	9348	PASS
173	174	0.00	2	0.9	1059	PASS
174	95	50	100	83.6	116923	PASS
175	174	5	9	7.5	8719	PASS
176	174	95	101	95.8	112043	PASS
177	176	5	9	6.8	7604	PASS