

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101824\
 Data File : VY019951.D
 Acq On : 18 Oct 2024 14:24
 Operator : SY/MD
 Sample : P4419-03
 Misc : 3.11g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Oct 18 23:33:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 16 05:44:48 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	2620	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.622	114	4317	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	2035	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	192	50.000	ug/l	# 0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.073	65	1755	54.402	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	= 108.800%	
35) Dibromofluoromethane	7.640	113	1477	51.847	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 103.700%	
50) Toluene-d8	10.109	98	4465	42.443	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 84.880%	
62) 4-Bromofluorobenzene	12.414	95	473	12.443	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	= 24.880%#	
Target Compounds						
					Qvalue	
6) Chloroethane	2.684	64	41	1.747	ug/l	# 42
10) Methyl Iodide	4.019	142	46	1.504	ug/l	# 42
11) Tert butyl alcohol	5.080	59	22	Below Cal	#	1
13) Acrolein	3.647	56	23	9.703	ug/l	# 15
15) Acrylonitrile	5.025	53	24	3.321	ug/l	# 1
16) Acetone	3.860	43	179	21.315	ug/l	# 36
18) Methyl Acetate	4.372	43	46	2.543	ug/l	# 46
25) 2-Butanone	6.884	43	62	5.516	ug/l	# 41
28) Bromochloromethane	7.329	49	80	2.960	ug/l	# 6
29) Tetrahydrofuran	7.232	42	102	15.892	ug/l	# 26
36) 1,1-Dichloropropene	7.707	75	215	5.239	ug/l	# 53
37) Ethyl Acetate	6.963	43	70	3.271	ug/l	# 67
38) Carbon Tetrachloride	7.719	117	172	3.909	ug/l	# 13
41) Methacrylonitrile	7.256	41	37	3.194	ug/l	# 15
43) Isopropyl Acetate	8.158	43	87	1.993	ug/l	# 47
45) 1,2-Dichloropropane	9.042	63	41	1.319	ug/l	# 43
48) Methyl methacrylate	9.225	41	41	2.136	ug/l	# 16
53) t-1,3-Dichloropropene	10.579	75	88	2.169	ug/l	# 45
58) 2-Chloroethyl Vinyl ether	9.658	63	50	3.345	ug/l	# 45
59) 2-Hexanone	10.701	43	62	3.899	ug/l	94
66) 1,1,1,2-Tetrachloroethane	11.469	131	22	1.397	ug/l	# 8
68) m/p-Xylenes	11.633	106	47	1.505	ug/l	# 1
74) N-amyl acetate	12.084	43	35	8.183	ug/l	# 64
76) 1,2,3-Trichloropropane	12.481	75	19	5.051	ug/l	# 100
78) n-propylbenzene	12.365	91	22	1.127	ug/l	# 53
81) trans-1,4-Dichloro-2-b...	12.408	75	194	208.190	ug/l	# 24
82) 4-Chlorotoluene	12.987	91	20	1.748	ug/l	# 39
85) sec-Butylbenzene	13.395	105	47	2.692	ug/l	# 56
90) Hexachloroethane	13.743	117	56	20.288	ug/l	# 12
92) 1,2-Dibromo-3-Chloropr...	14.017	75	46	100.443	ug/l	# 1
95) Naphthalene	15.151	128	22	3.421	ug/l	# 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101824\
Data File : VY019951.D
Acq On : 18 Oct 2024 14:24
Operator : SY/MD
Sample : P4419-03
Misc : 3.11g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Oct 18 23:33:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 16 05:44:48 2024
Response via : Initial Calibration




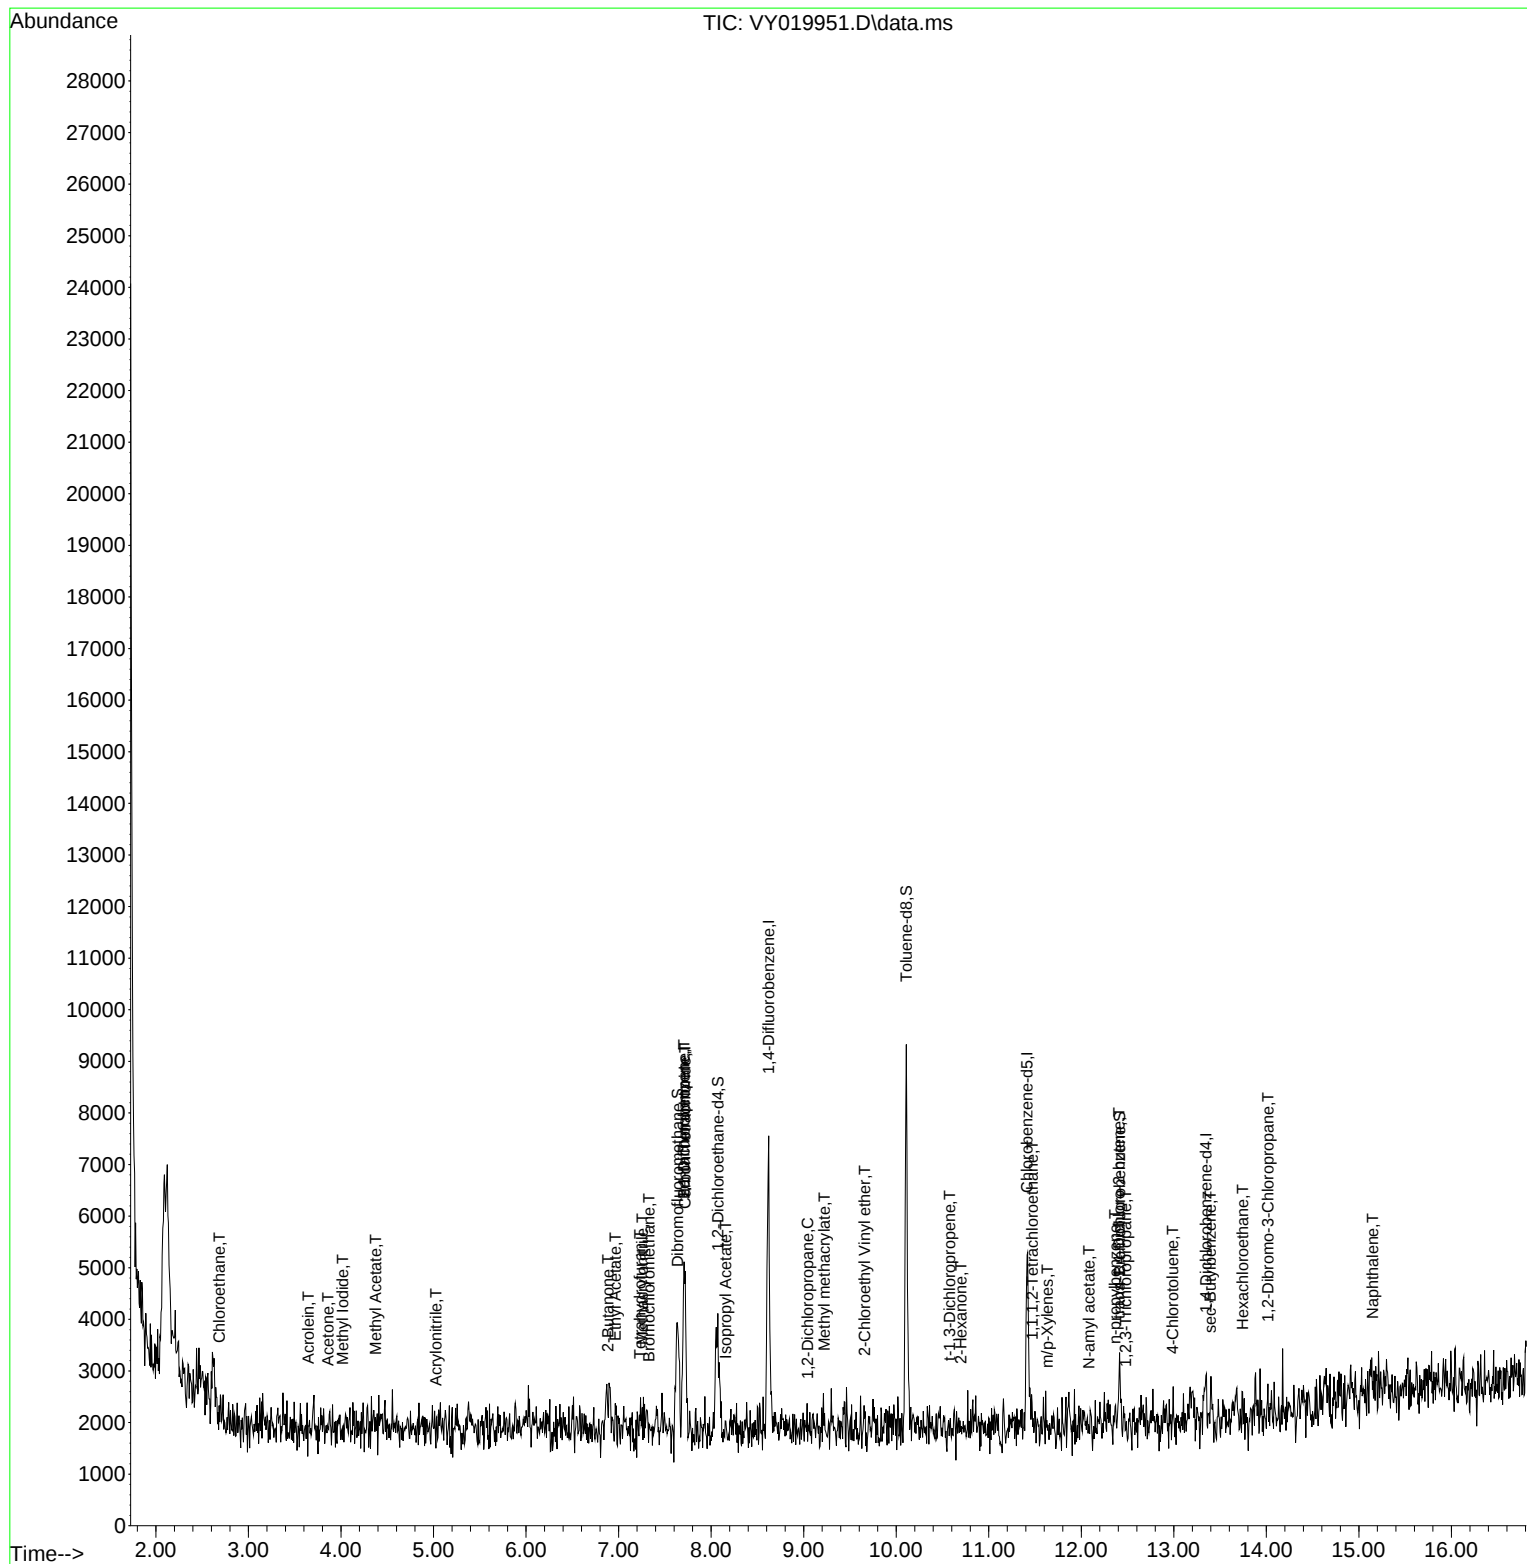




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 2620
Ion Ratio Lower Upper
168 100
99 59.2 39.1 58.7#

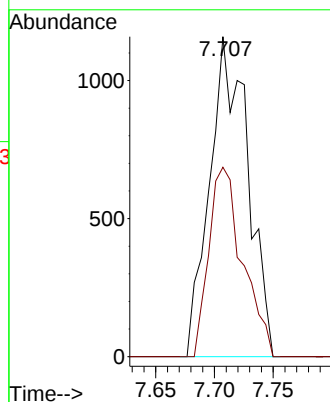

#6
Chloroethane
Concen: 1.747 ug/l
RT: 2.684 min Scan# 158
Delta R.T. -0.055 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24


Tgt Ion: 64 Resp: 41
Ion Ratio Lower Upper
64 100
66 0.0 26.1 39.1#

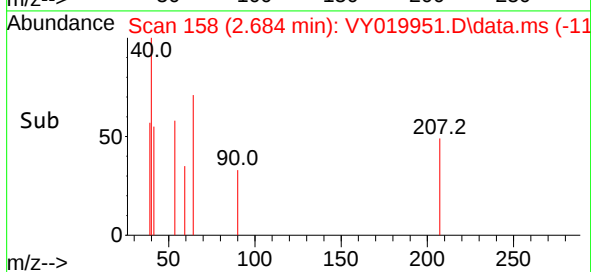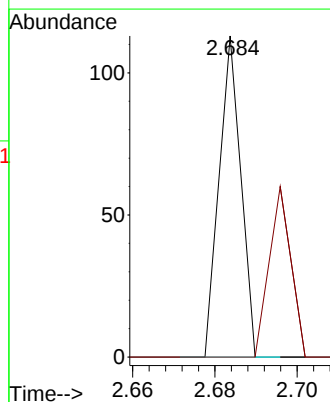






#10
Methyl Iodide
Concen: 1.504 ug/l
RT: 4.019 min Scan# 31
Delta R.T. 0.012 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:142 Resp: 46
Ion Ratio Lower Upper
142 100
127 0.0 32.8 49.2#
141 0.0 11.4 17.2#

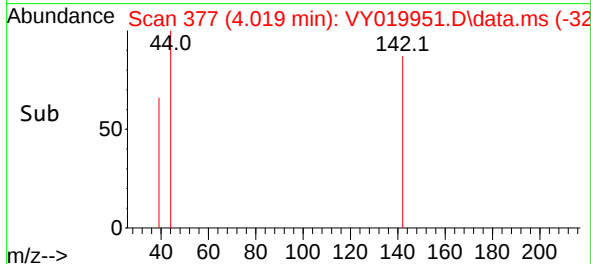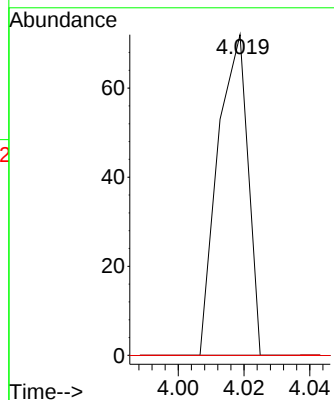

#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.080 min Scan# 551
Delta R.T. 0.220 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 59 Resp: 22
Ion Ratio Lower Upper
59 100
57 100.0 3.0 4.6#

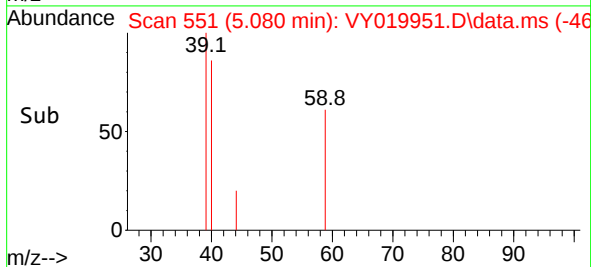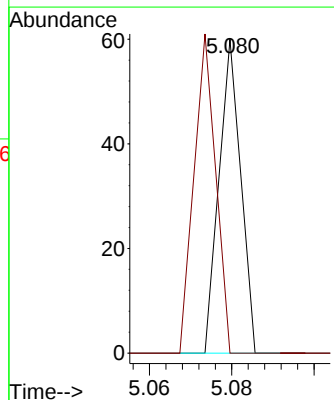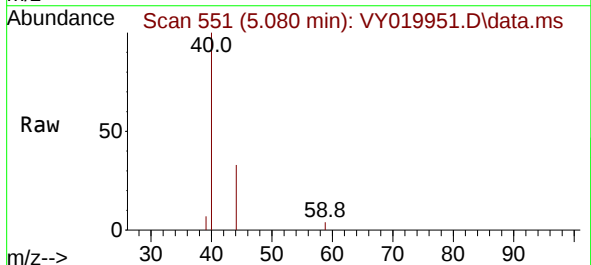



#13

Acrolein

Concen: 9.703 ug/l

RT: 3.647 min Scan# 317

Delta R.T. -0.006 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 56 Resp: 23

Ion Ratio Lower Upper

56 100

55 0.0 55.7 83.5#

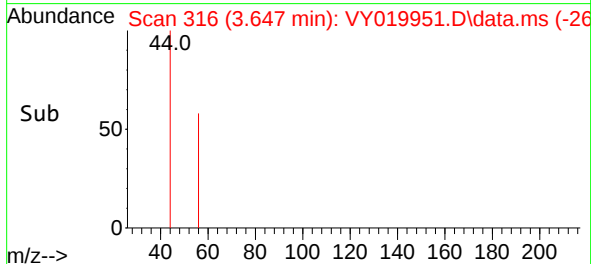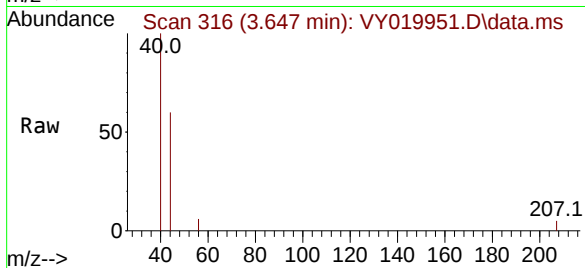

#15

Acrylonitrile

Concen: 3.321 ug/l

RT: 5.025 min Scan# 542

Delta R.T. -0.030 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Tgt Ion: 53 Resp: 24


Ion Ratio Lower Upper

53 100

52 0.0 64.7 97.1#

51 141.7 28.4 42.6#


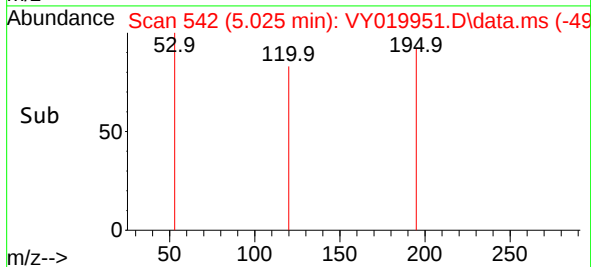

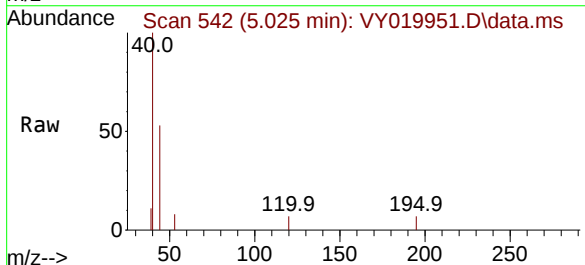




#16
Acetone
Concen: 21.315 ug/l
RT: 3.860 min Scan# 31
Delta R.T. -0.012 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 179
Ion Ratio Lower Upper
43 100
58 0.0 31.7 47.5#

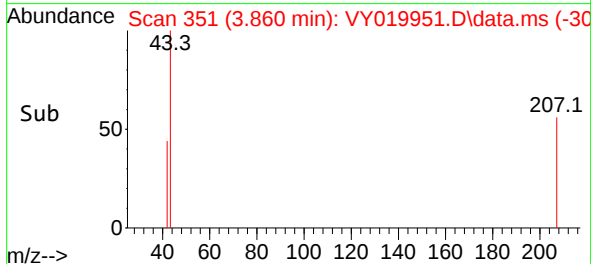

#18
Methyl Acetate
Concen: 2.543 ug/l
RT: 4.372 min Scan# 435
Delta R.T. -0.012 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 43 Resp: 46
Ion Ratio Lower Upper
43 100
74 0.0 23.3 34.9#

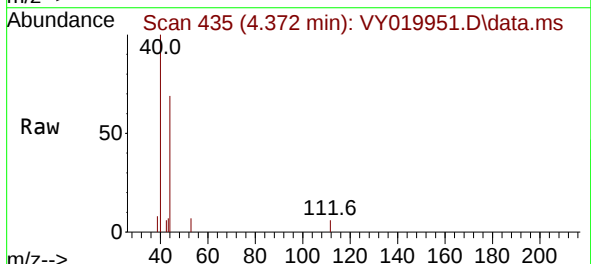

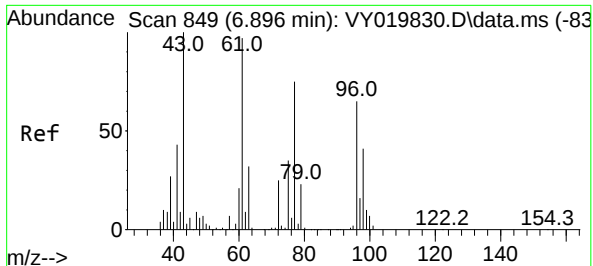

#25

2-Butanone

Concen: 5.516 ug/l

RT: 6.884 min Scan# 84

Delta R.T. -0.006 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 43 Resp: 62

Ion Ratio Lower Upper

43 100

72 0.0 27.3 40.9#

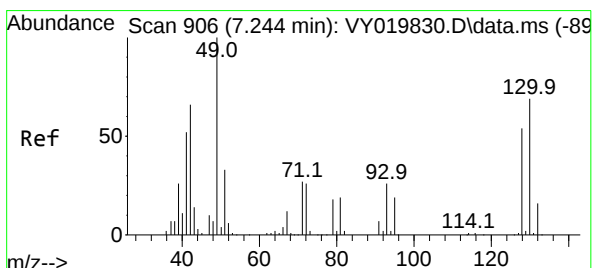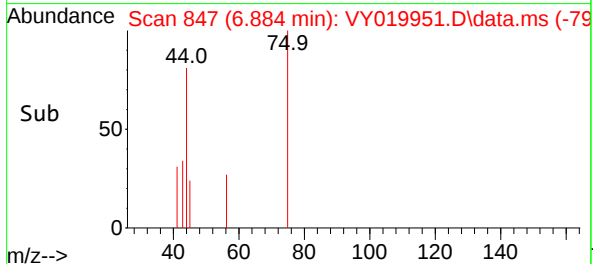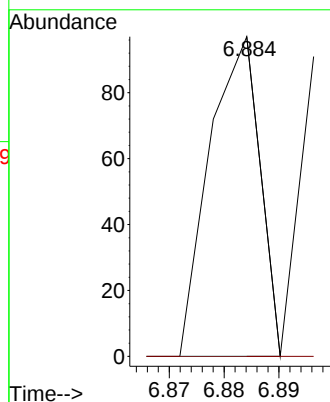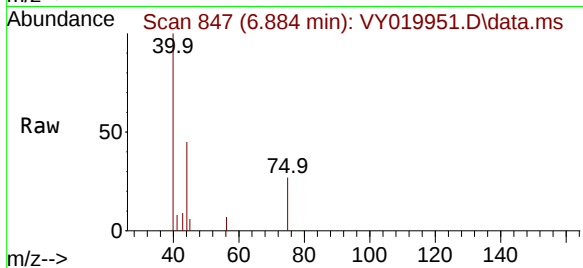

#28

Bromochloromethane

Concen: 2.960 ug/l

RT: 7.329 min Scan# 920

Delta R.T. 0.086 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Tgt Ion: 49 Resp: 80


Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.6

130 0.0 72.7 109.1#

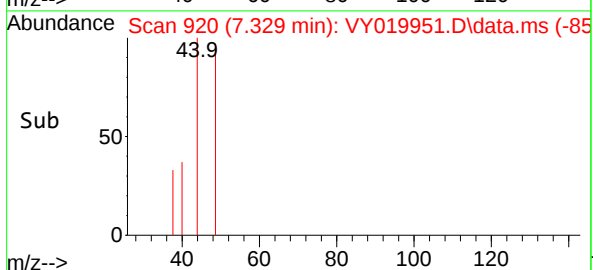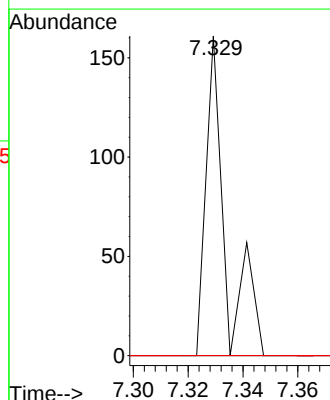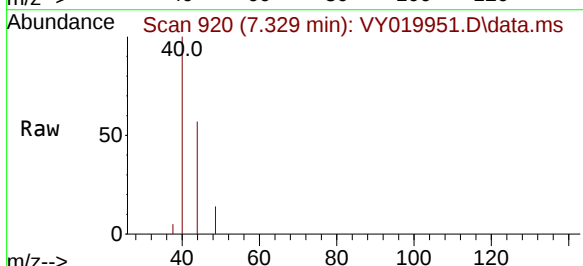

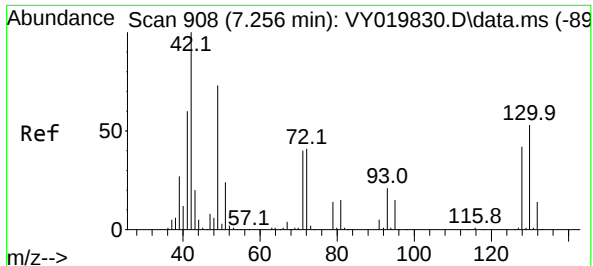

#29

Tetrahydrofuran

Concen: 15.892 ug/l

RT: 7.232 min Scan# 90

Delta R.T. -0.030 min


Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Instrument :

MSVOA_Y

ClientSampleId :

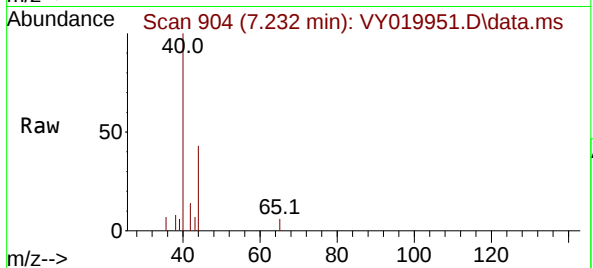

Tgt Ion:	42	Resp:	102
Ion	Ratio	Lower	Upper
42	100		
72	0.0	43.0	64.4#
71	0.0	40.8	61.2#

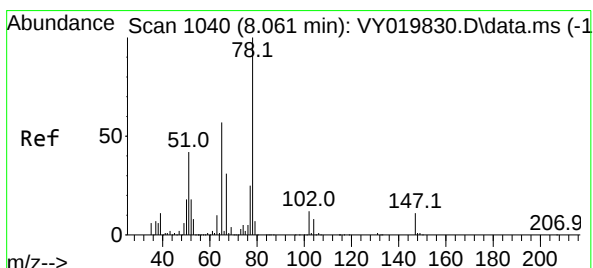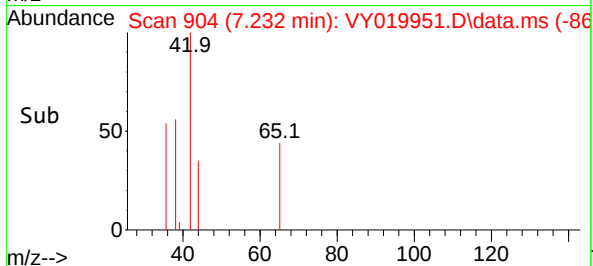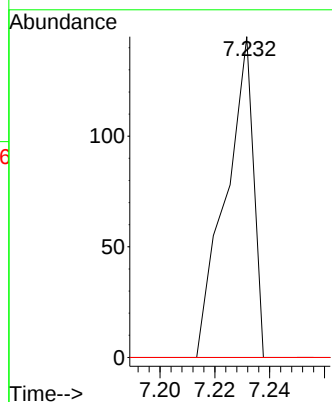

#33

1,2-Dichloroethane-d4

Concen: 54.402 ug/l




RT: 8.073 min Scan# 1042


Delta R.T. 0.012 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Tgt Ion:	65	Resp:	1755
Ion	Ratio	Lower	Upper
65	100		
67	46.4	0.0	109.6

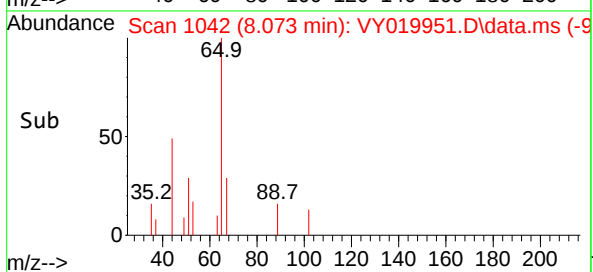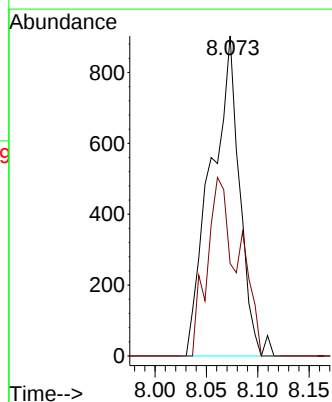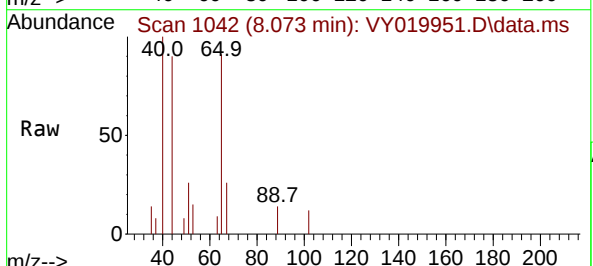



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.622 min Scan# 1131

Delta R.T. 0.006 min

Lab File: VY019951.D





Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:114	Resp:	4317
Ion	Ratio	Lower Upper
114	100	
63	31.1	0.0 35.0
88	17.6	0.0 27.2

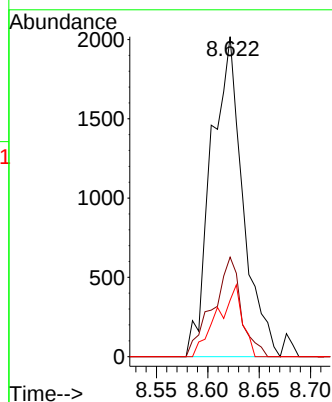

#35

Dibromofluoromethane

Concen: 51.847 ug/l




RT: 7.640 min Scan# 971


Delta R.T. 0.006 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Tgt Ion:113	Resp:	1477
Ion	Ratio	Lower Upper
113	100	
111	110.3	82.2 123.4
192	7.9	15.9 23.9#

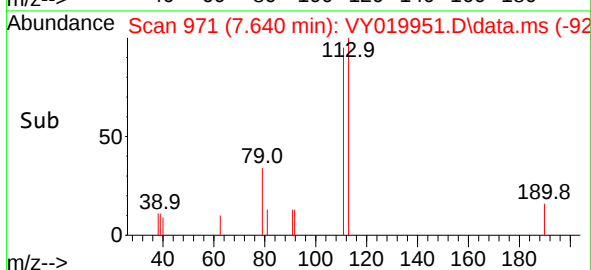



#36

1,1-Dichloropropene

Concen: 5.239 ug/l

RT: 7.707 min Scan# 91

Delta R.T. -0.128 min


Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y

ClientSampleId :






Tgt Ion: 75 Resp: 215

Ion Ratio Lower Upper

75 100

110 14.9 19.0 57.0#

77 0.0 25.3 37.9#

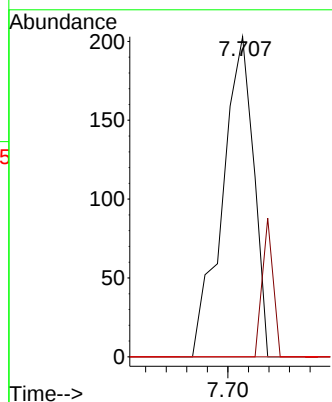

#37

Ethyl Acetate

Concen: 3.271 ug/l

RT: 6.963 min Scan# 860

Delta R.T. -0.018 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Tgt Ion: 43 Resp: 70


Ion Ratio Lower Upper

43 100

61 0.0 12.6 19.0#


70 0.0 7.8 11.8#

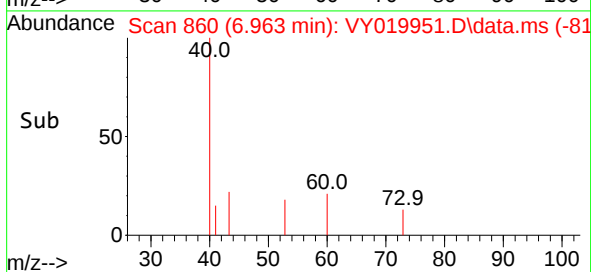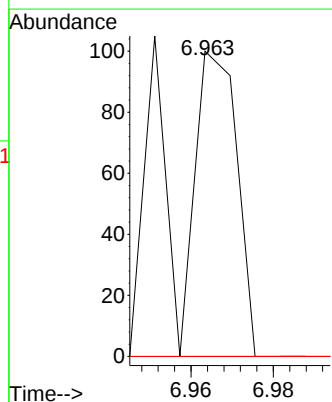



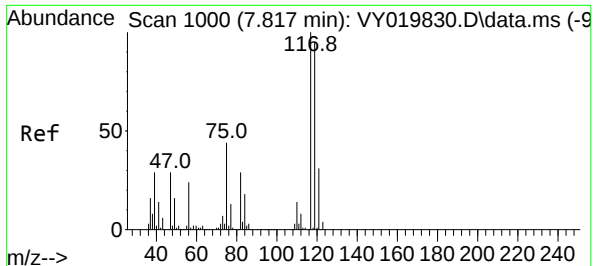


#38
Carbon Tetrachloride
Concen: 3.909 ug/l
RT: 7.719 min Scan# 908
Delta R.T. -0.097 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24


Instrument :
MSVOA_Y
ClientSampleId :

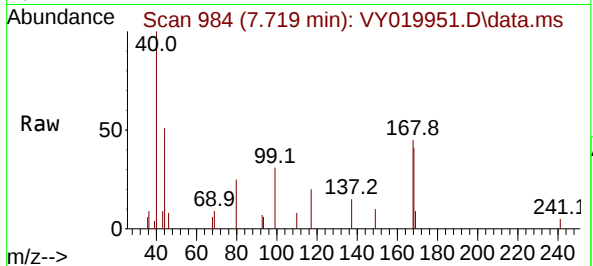



Tgt Ion:117 Resp: 172
Ion Ratio Lower Upper
117 100
119 0.0 75.8 113.6#
121 0.0 24.0 36.0#

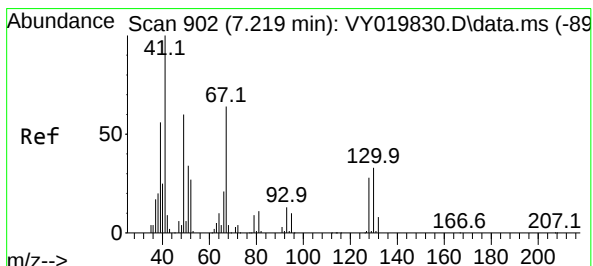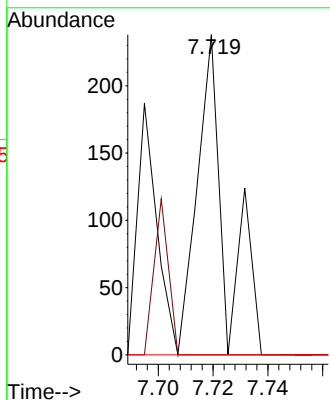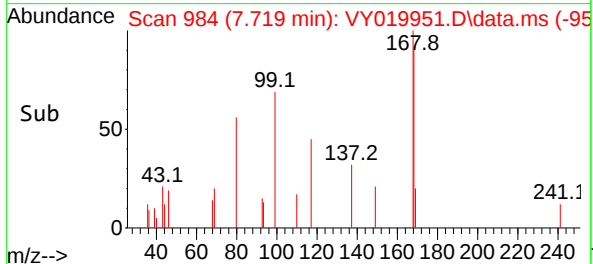


#41
Methacrylonitrile
Concen: 3.194 ug/l
RT: 7.256 min Scan# 908
Delta R.T. 0.037 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

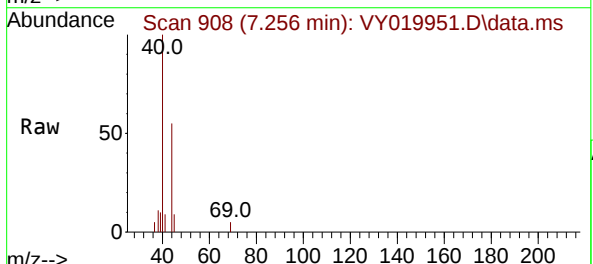

Tgt Ion: 41 Resp: 37
Ion Ratio Lower Upper
41 100
39 0.0 48.0 72.0#
67 0.0 75.1 112.7#
52 0.0 29.8 44.6#

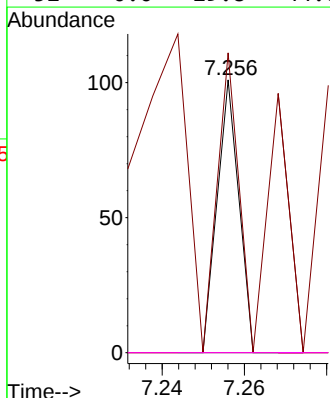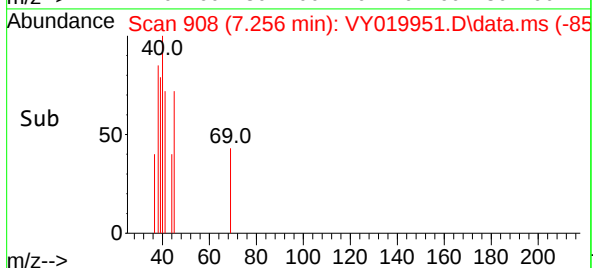

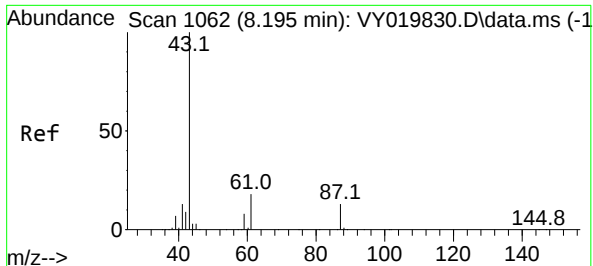

#43

Isopropyl Acetate

Concen: 1.993 ug/l

RT: 8.158 min Scan# 1056

Delta R.T. -0.036 min


Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Instrument :

MSVOA_Y

ClientSampleId :

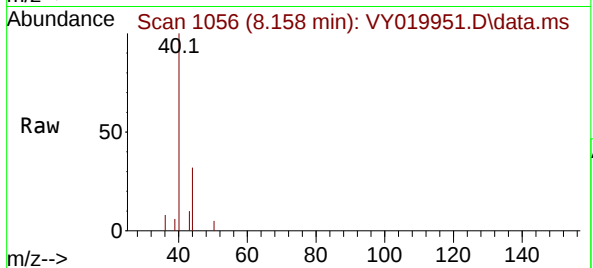

Tgt Ion:	43	Resp:	87
Ion	Ratio	Lower	Upper
43	100		
61	0.0	27.9	41.9#
87	0.0	13.1	19.7#

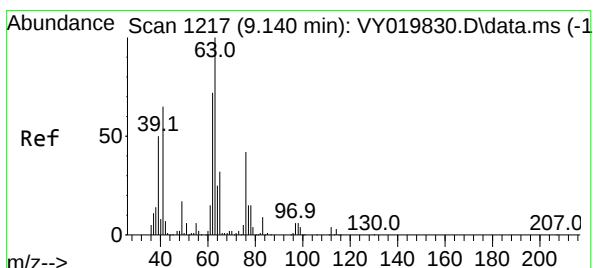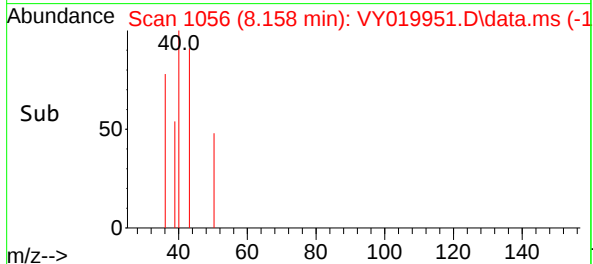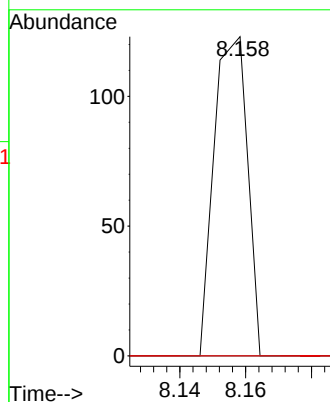

#45

1,2-Dichloropropane

Concen: 1.319 ug/l




RT: 9.042 min Scan# 1201


Delta R.T. -0.097 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Tgt Ion:	63	Resp:	41
Ion	Ratio	Lower	Upper
63	100		
65	0.0	25.4	38.2#


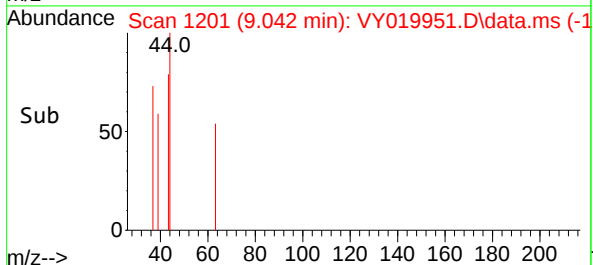
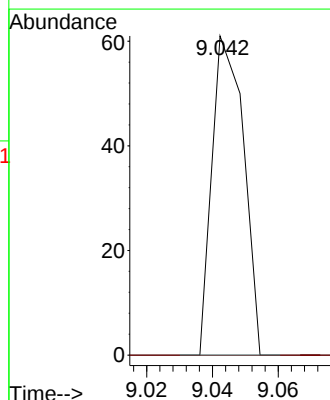
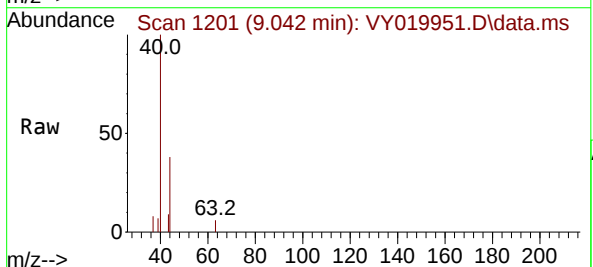




#48
Methyl methacrylate
Concen: 2.136 ug/l
RT: 9.225 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 41 Resp: 41
Ion Ratio Lower Upper
41 100
69 0.0 84.1 126.1#
39 90.2 43.6 65.4#

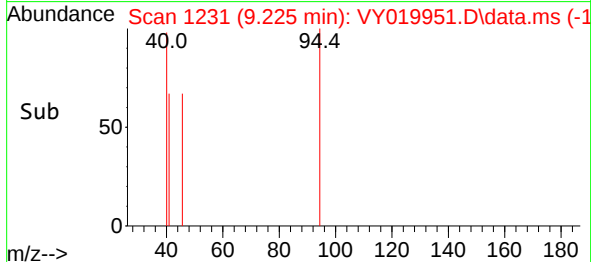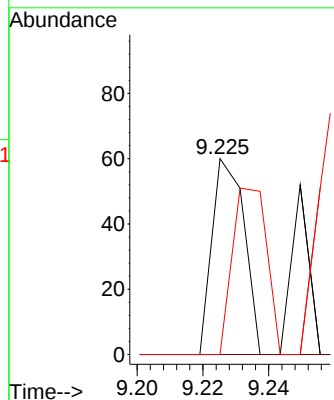

#50
Toluene-d8
Concen: 42.443 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 98 Resp: 4465
Ion Ratio Lower Upper
98 100
100 66.6 52.0 78.0


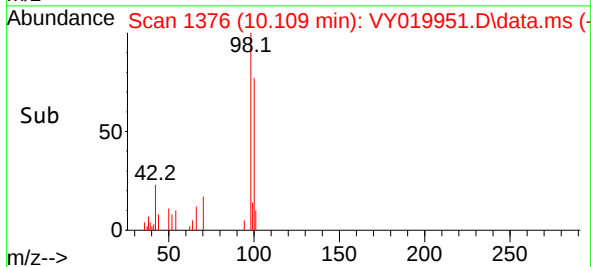
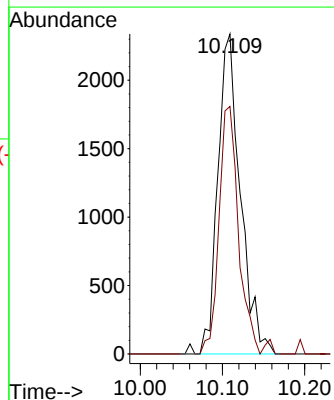
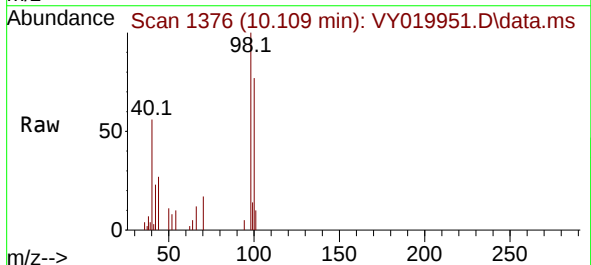


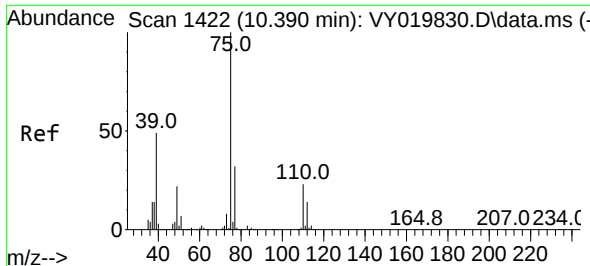

#53
t-1,3-Dichloropropene
Concen: 2.169 ug/l
RT: 10.579 min Scan# 1422
Delta R.T. 0.183 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 88
Ion Ratio Lower Upper
75 100
77 0.0 24.1 36.1#

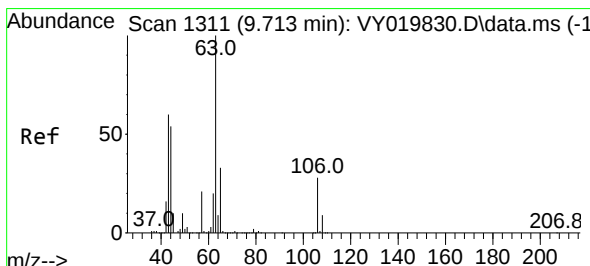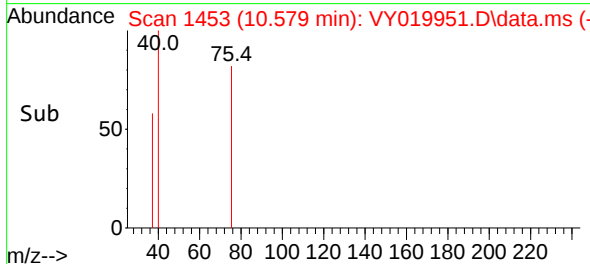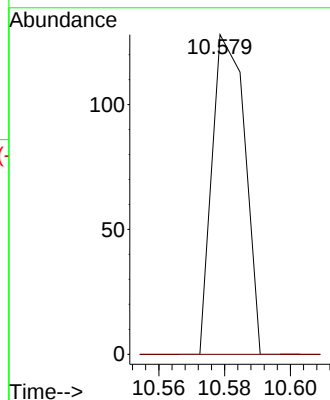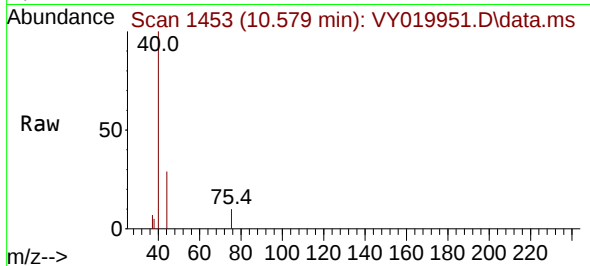

#58
2-Chloroethyl Vinyl ether
Concen: 3.345 ug/l
RT: 9.658 min Scan# 1302
Delta R.T. -0.055 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 63 Resp: 50
Ion Ratio Lower Upper
63 100
106 0.0 23.7 35.5#


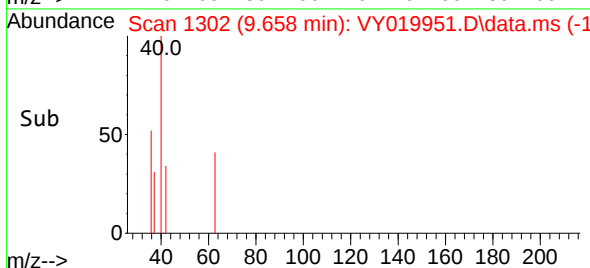
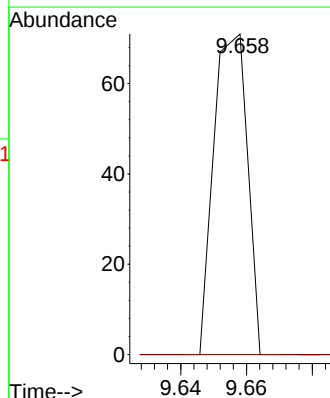
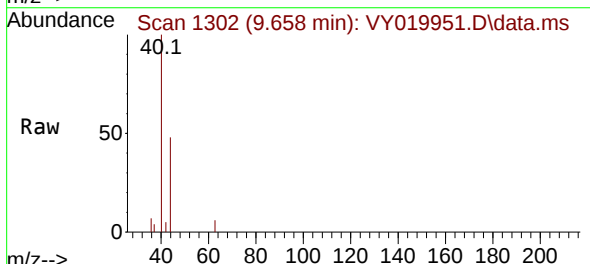




#59
2-Hexanone
Concen: 3.899 ug/l
RT: 10.701 min Scan# 14
Delta R.T. -0.061 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 62
Ion Ratio Lower Upper
43 100
58 58.1 31.4 94.0

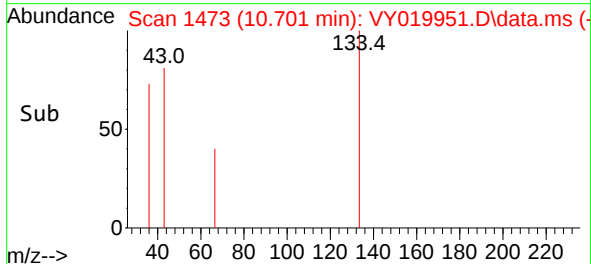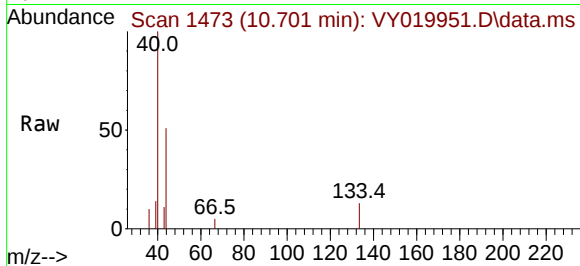

#62
4-Bromofluorobenzene
Concen: 12.443 ug/l
RT: 12.414 min Scan# 1754
Delta R.T. 0.006 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 95 Resp: 473
Ion Ratio Lower Upper
95 100
174 54.3 0.0 175.6
176 45.2 0.0 171.4

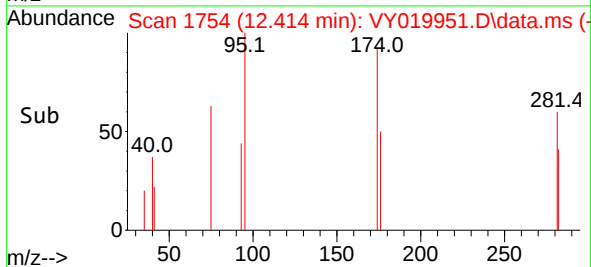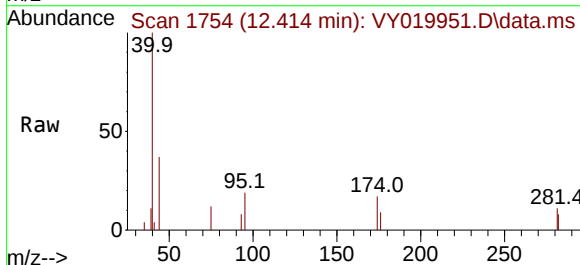



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min


Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Instrument :

MSVOA_Y

ClientSampleId :



Tgt Ion:	117	Resp:	2035
Ion Ratio	Lower	Upper	
117	100		
82	48.5	42.4	63.6
119	47.6	25.9	38.9#

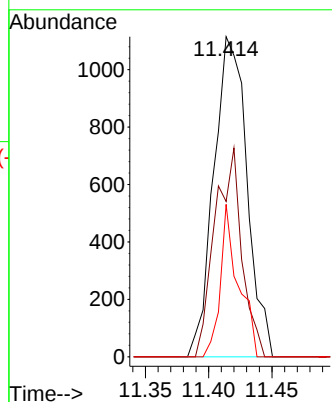

#66

1,1,1,2-Tetrachloroethane

Concen: 1.397 ug/l




RT: 11.469 min Scan# 1599


Delta R.T. -0.049 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Tgt Ion:	131	Resp:	22
Ion Ratio	Lower	Upper	
131	100		
133	0.0	47.8	143.3#
119	0.0	34.1	102.2#


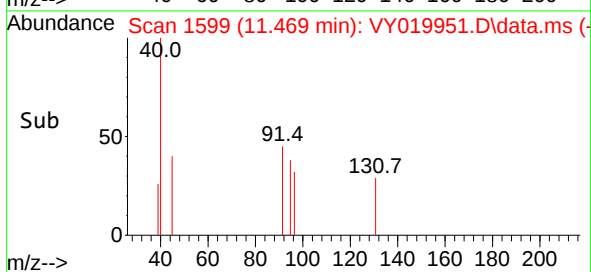






#68
m/p-Xylenes
Concen: 1.505 ug/l
RT: 11.633 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:106 Resp: 47
Ion Ratio Lower Upper
106 100
91 0.0 156.0 234.0#

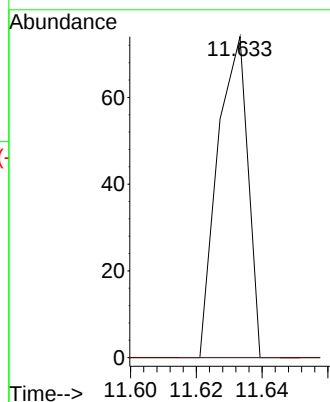

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion:152 Resp: 192
Ion Ratio Lower Upper
152 100
115 101.6 28.2 84.7#
150 285.9 0.0 345.6

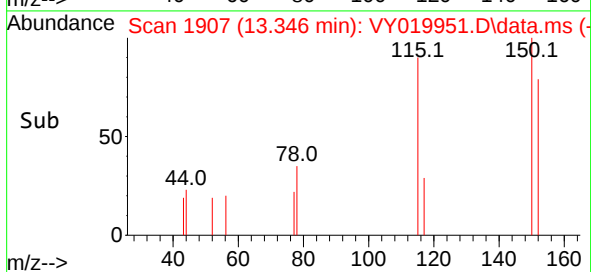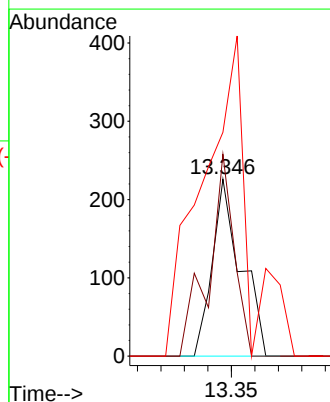



#74

N-amy1 acetate

Concen: 8.183 ug/l

RT: 12.084 min Scan# 1

Delta R.T. 0.012 min


Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y

ClientSampleId :

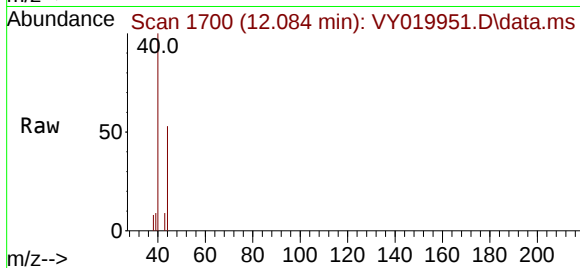

Tgt Ion: 43 Resp: 35




Ion Ratio Lower Upper

43 100

70 62.9 41.4 62.2#

55 0.0 23.3 34.9#

61 0.0 22.6 33.8#

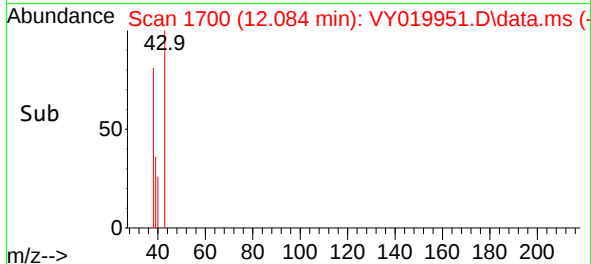

#76

1,2,3-Trichloropropane

Concen: 5.051 ug/l

RT: 12.481 min Scan# 1765

Delta R.T. -0.079 min

Lab File: VY019951.D




Acq: 18 Oct 2024 14:24


Tgt Ion: 75 Resp: 19

Ion Ratio Lower Upper

75 100

77 0.0 0.0 0.0

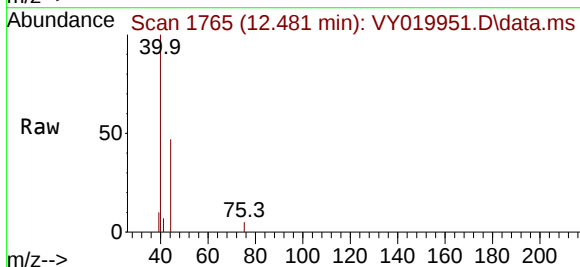



#78

n-propylbenzene

Concen: 1.127 ug/l

RT: 12.365 min Scan# 11

Delta R.T. -0.231 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 91 Resp: 22

Ion Ratio Lower Upper

91 100

120 0.0 11.5 34.4#

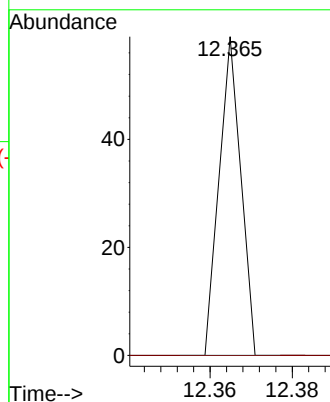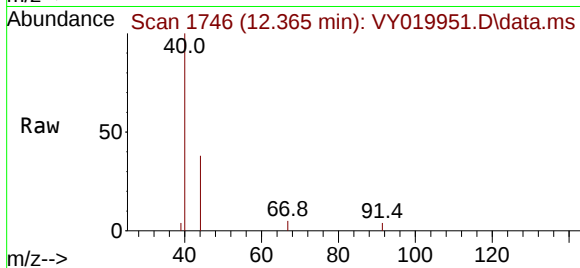

#81

trans-1,4-Dichloro-2-butene

Concen: 208.190 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.104 min

Lab File: VY019951.D

Acq: 18 Oct 2024 14:24




Tgt Ion: 75 Resp: 194


Ion Ratio Lower Upper

75 100

53 11.9 66.8 100.2#

89 0.0 35.8 53.6#


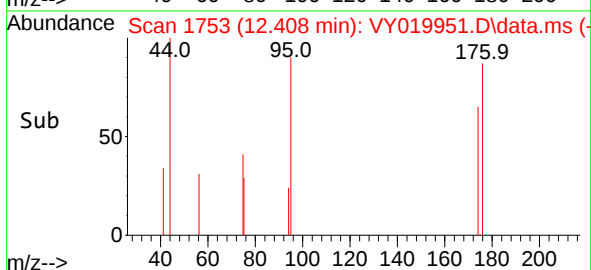
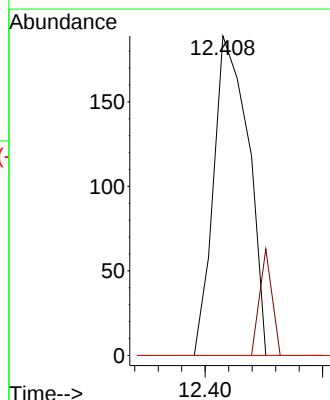
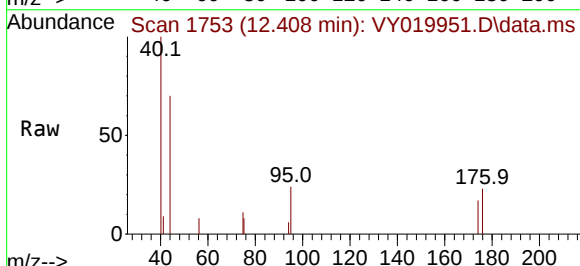




#82
4-Chlorotoluene
Concen: 1.748 ug/l
RT: 12.987 min Scan# 11
Delta R.T. 0.208 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 20
Ion Ratio Lower Upper
91 100
126 0.0 17.6 52.9#

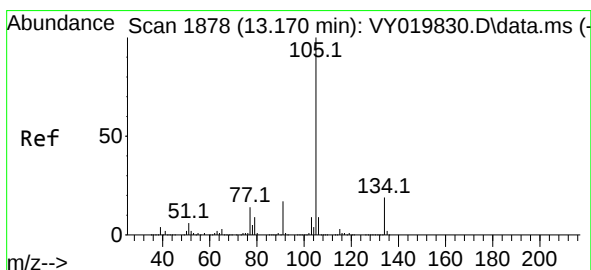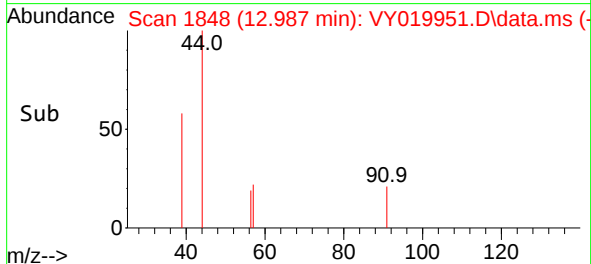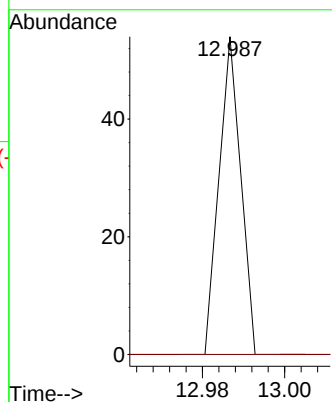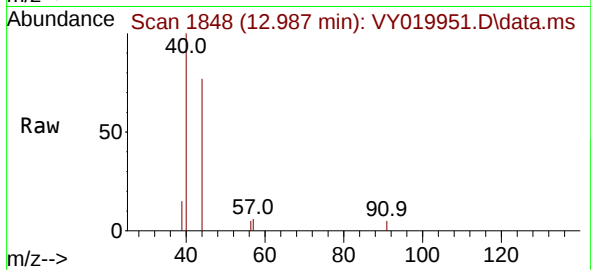

#85
sec-Butylbenzene
Concen: 2.692 ug/l
RT: 13.395 min Scan# 1915
Delta R.T. 0.220 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Tgt Ion: 105 Resp: 47
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#


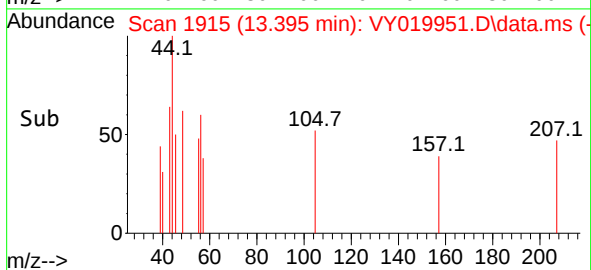
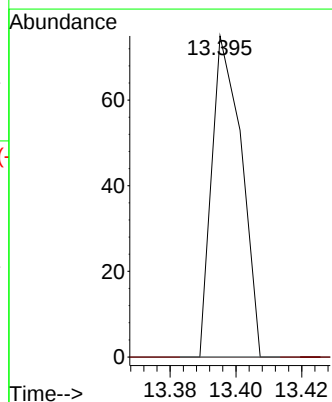
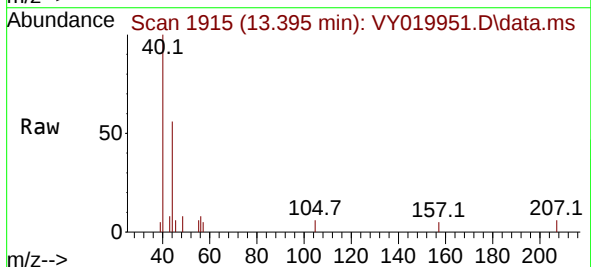




#90
Hexachloroethane
Concen: 20.288 ug/l
RT: 13.743 min Scan# 1994
Delta R.T. -0.140 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:117 Resp: 56
Ion Ratio Lower Upper
117 100
201 0.0 37.4 112.2#

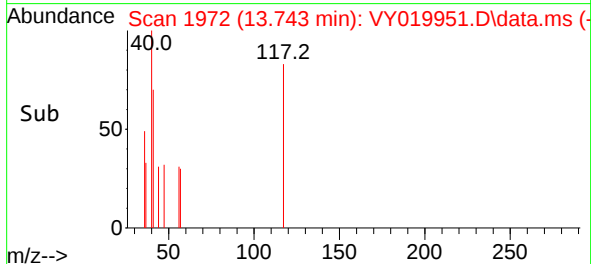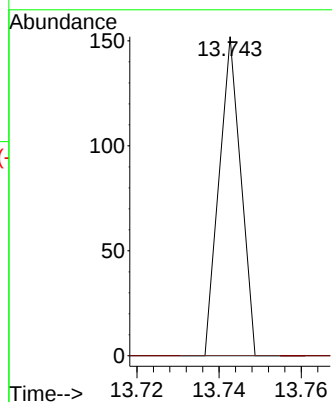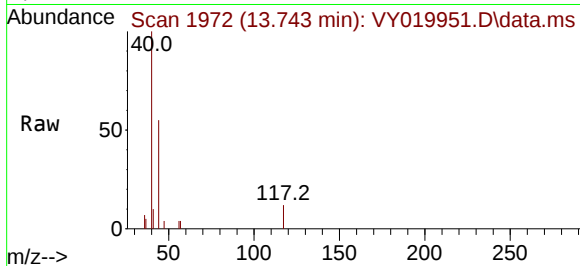

#92
1,2-Dibromo-3-Chloropropane
Concen: 100.443 ug/l
RT: 14.017 min Scan# 2017
Delta R.T. -0.256 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24


Tgt Ion: 75 Resp: 46
Ion Ratio Lower Upper
75 100
155 0.0 48.6 145.8#
157 0.0 62.7 188.2#

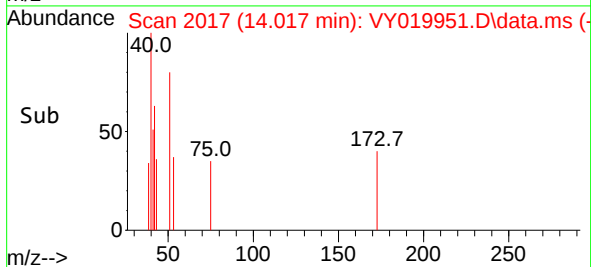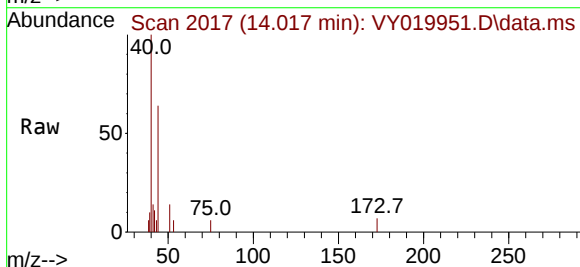



#95
Naphthalene
Concen: 3.421 ug/l
RT: 15.151 min Scan# 21
Delta R.T. 0.006 min
Lab File: VY019951.D
Acq: 18 Oct 2024 14:24

Instrument :
MSVOA_Y
ClientSampleId :

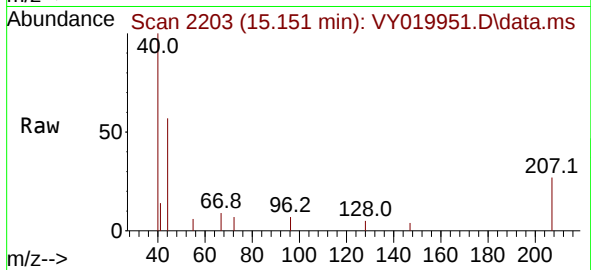

Tgt Ion:128 Resp: 22
Ion Ratio Lower Upper
128 100
127 0.0 10.6 16.0#
129 0.0 8.6 13.0#

