
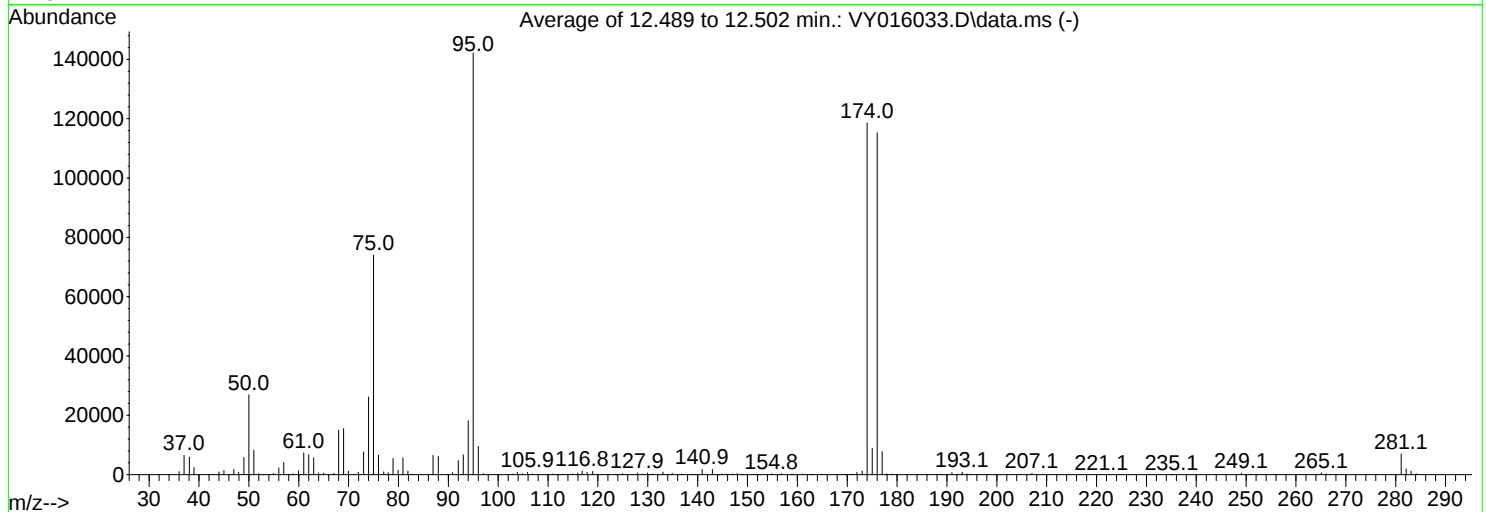


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101923\
Data File : VY016033.D
Acq On : 19 Oct 2023 08:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101823S.M
Title : SW846 8260
Last Update : Thu Oct 19 03:15:44 2023

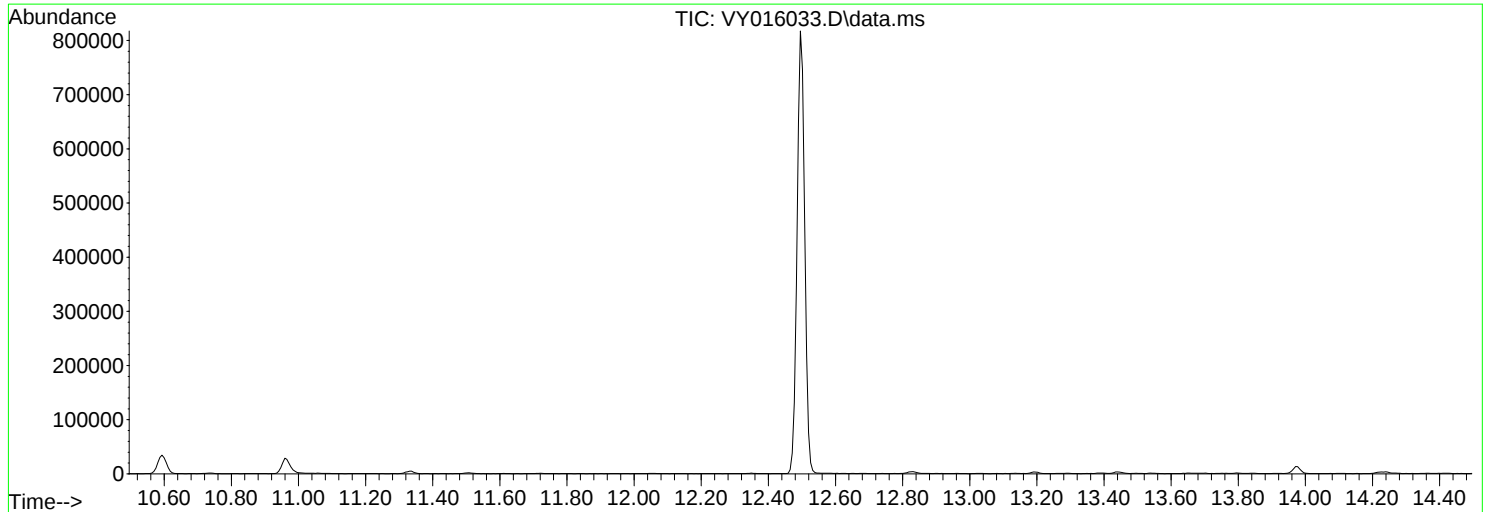

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	26928	PASS
75	95	30	60	52.0	73944	PASS
95	95	100	100	100.0	142203	PASS
96	95	5	9	6.7	9553	PASS
173	174	0.00	2	1.0	1187	PASS
174	95	50	100	83.4	118565	PASS
175	174	5	9	7.5	8899	PASS
176	174	95	101	97.2	115285	PASS
177	176	5	9	6.7	7780	PASS