

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102022\
 Data File : VY011023.D
 Acq On : 20 Oct 2022 14:27
 Operator : KP/MD
 Sample : N5193-03
 Misc : 3.76g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 LSP-SS-02-01-03

Quant Time: Oct 20 22:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 01:42:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	286556	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	506208	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	345321	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	90638	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	189617	71.835	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 143.680%	
35) Dibromofluoromethane	7.716	113	189283	67.850	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 135.700%	
50) Toluene-d8	10.179	98	570675	53.992	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 107.980%	
62) 4-Bromofluorobenzene	12.477	95	135708	35.346	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 70.700%	
Target Compounds						
16) Acetone	3.948	43	17254	22.509	ug/l	# 88
17) Carbon Disulfide	4.192	76	20938	2.627	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102022\
Data File : VY011023.D
Acq On : 20 Oct 2022 14:27
Operator : KP/MD
Sample : N5193-03
Misc : 3.76g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03

Quant Time: Oct 20 22:23:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 01:42:42 2022
Response via : Initial Calibration




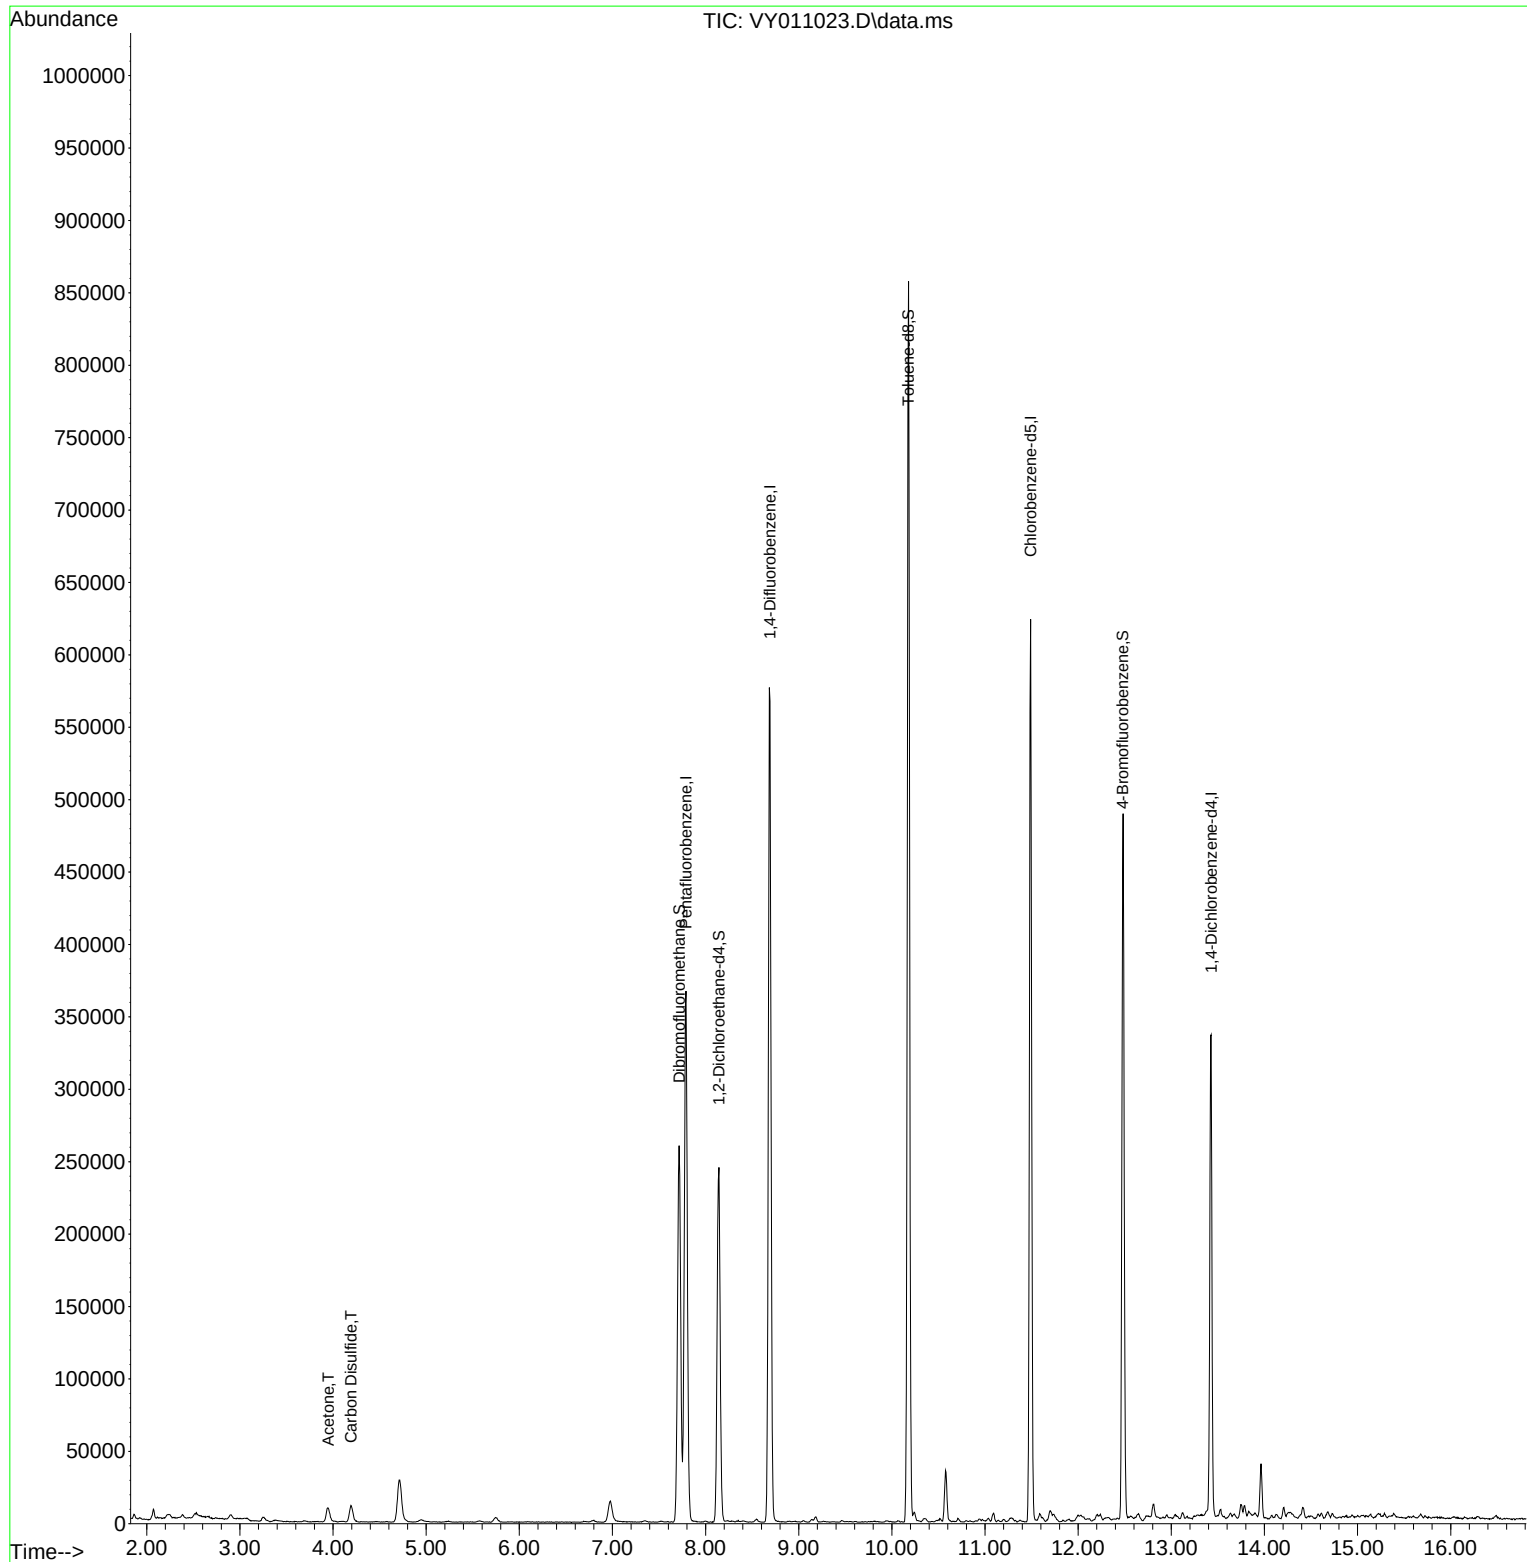


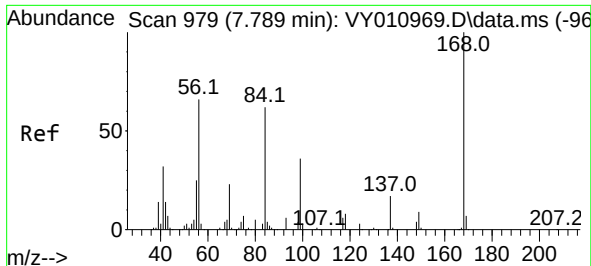

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27




Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03


Tgt Ion:168 Resp: 286556
Ion Ratio Lower Upper
168 100
99 54.1 46.9 70.3

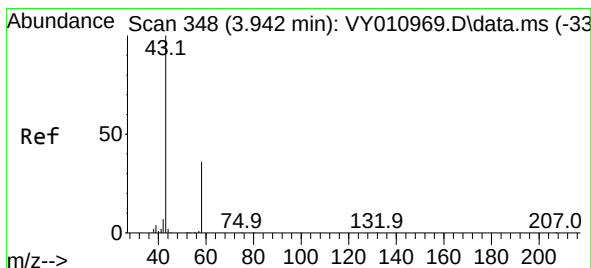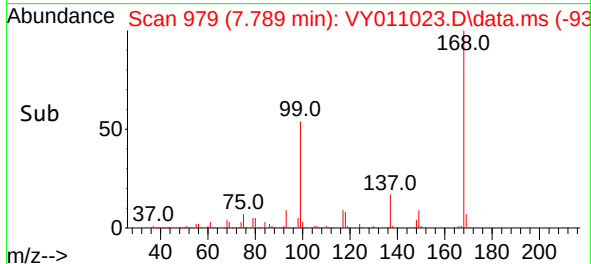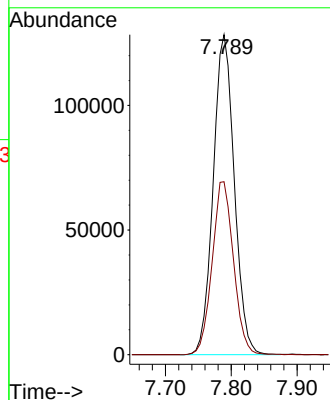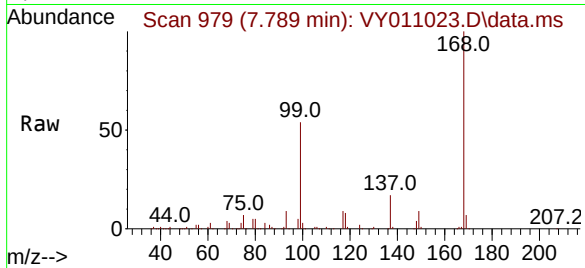

#16
Acetone
Concen: 22.509 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Tgt Ion: 43 Resp: 17254
Ion Ratio Lower Upper
43 100
58 33.9 22.0 33.0#


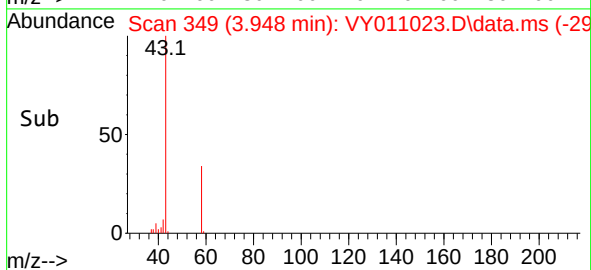
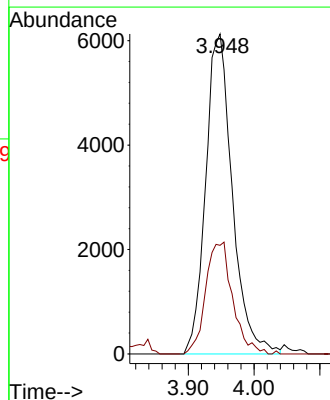
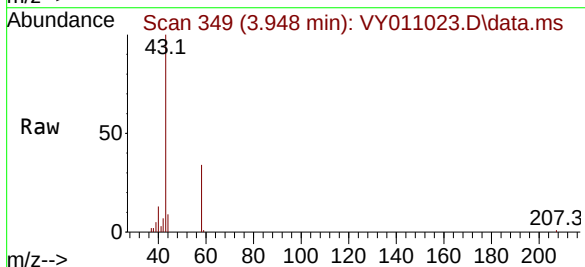


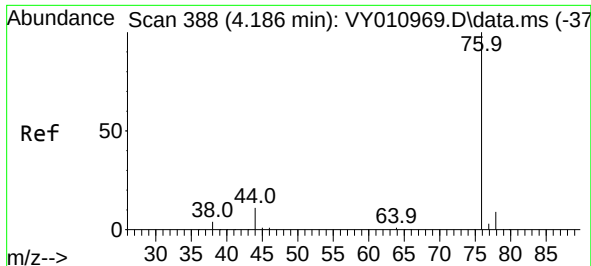

#17
Carbon Disulfide
Concen: 2.627 ug/l
RT: 4.192 min Scan# 31
Delta R.T. 0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27




Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03


Tgt Ion: 76 Resp: 20938
Ion Ratio Lower Upper
76 100
78 8.9 7.4 11.0

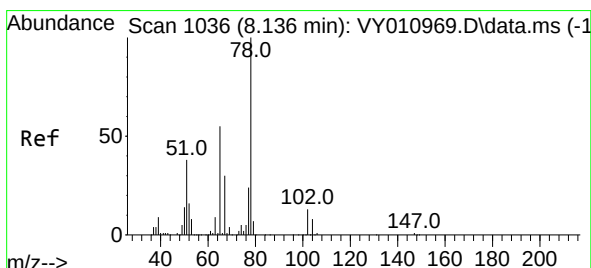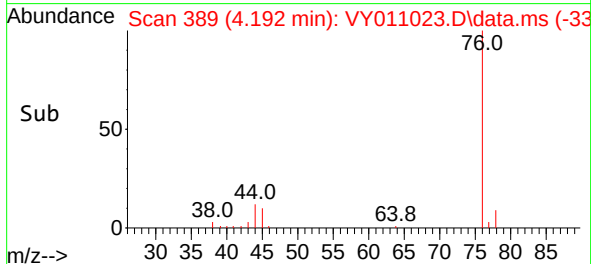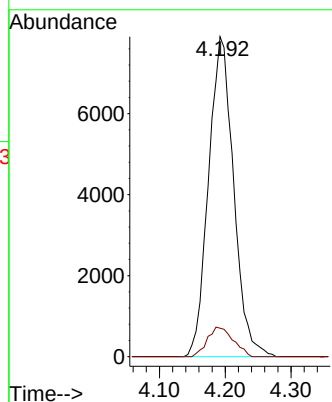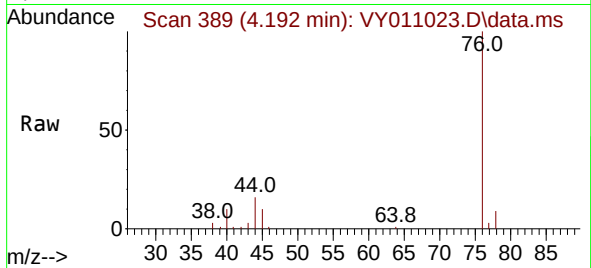

#33
1,2-Dichloroethane-d4
Concen: 71.835 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Tgt Ion: 65 Resp: 189617
Ion Ratio Lower Upper
65 100
67 54.5 0.0 99.4


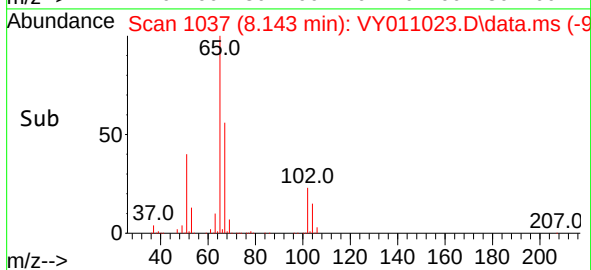
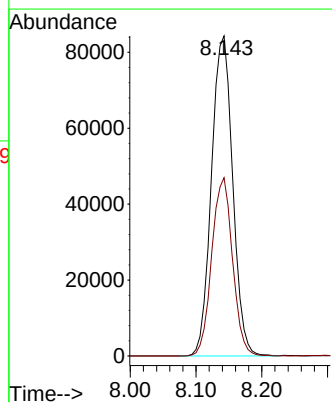
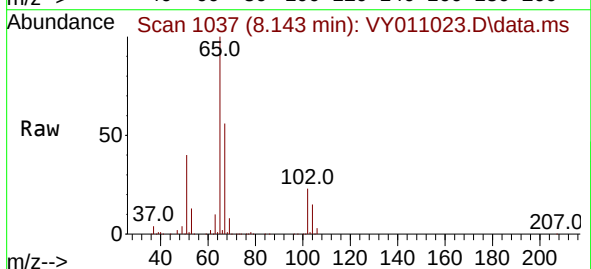


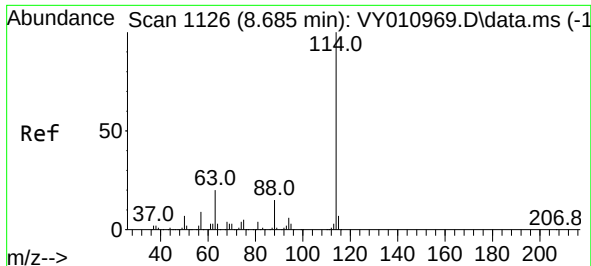

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27




Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03


Tgt Ion:114 Resp: 506208
Ion Ratio Lower Upper
114 100
63 18.7 0.0 43.2
88 14.6 0.0 31.8

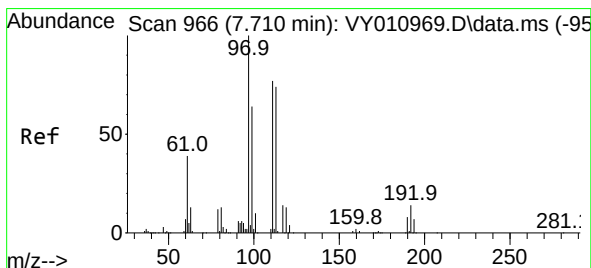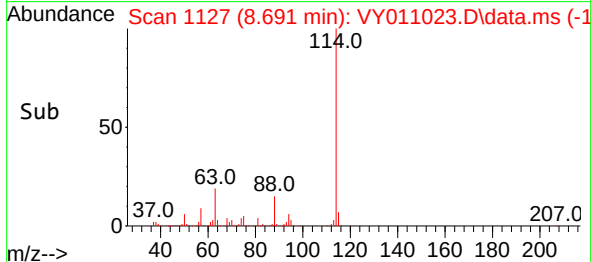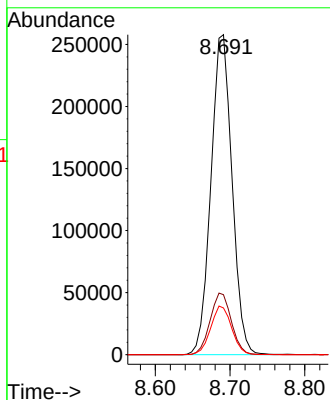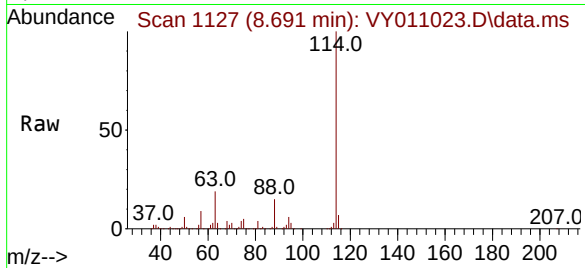

#35
Dibromofluoromethane
Concen: 67.850 ug/l
RT: 7.716 min Scan# 967
Delta R.T. 0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Tgt Ion:113 Resp: 189283
Ion Ratio Lower Upper
113 100
111 102.6 82.6 124.0
192 19.9 17.6 26.4


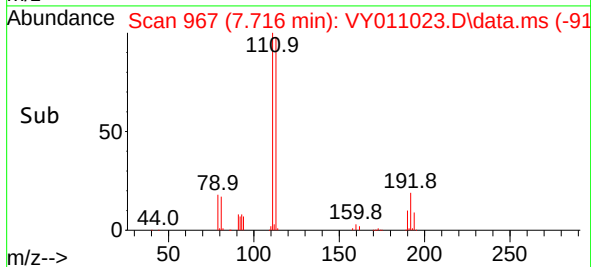
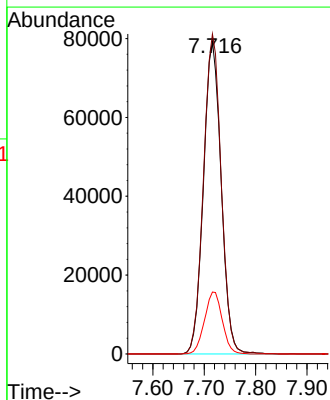
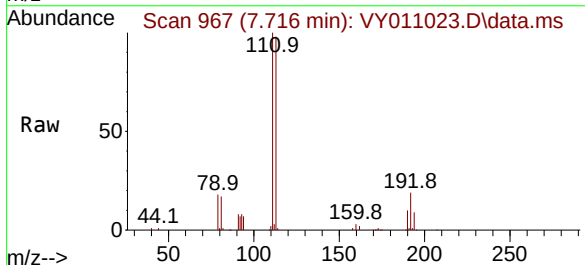


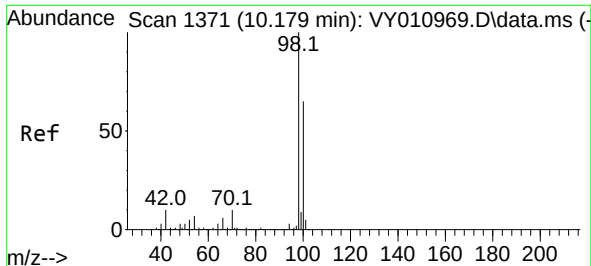

#50
Toluene-d8
Concen: 53.992 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27




Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03


Tgt Ion: 98 Resp: 570675
Ion Ratio Lower Upper
98 100
100 65.1 50.2 75.2

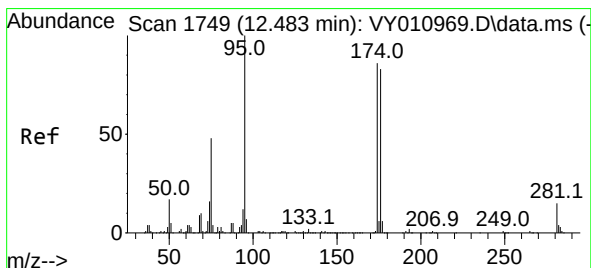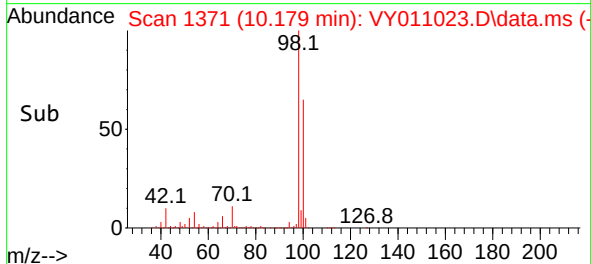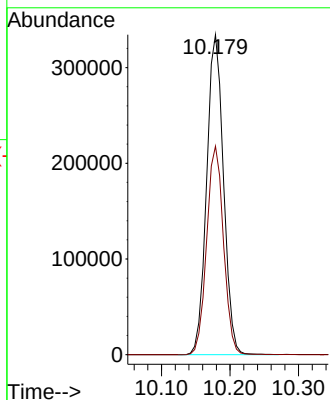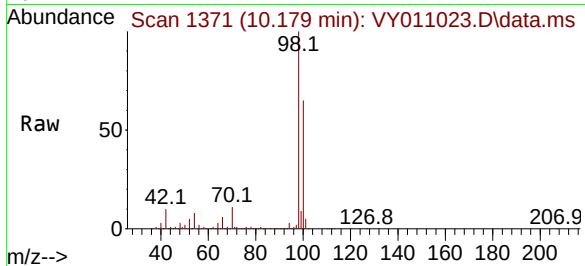

#62
4-Bromofluorobenzene
Concen: 35.346 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Tgt Ion: 95 Resp: 135708
Ion Ratio Lower Upper
95 100
174 84.0 0.0 177.0
176 80.2 0.0 175.8


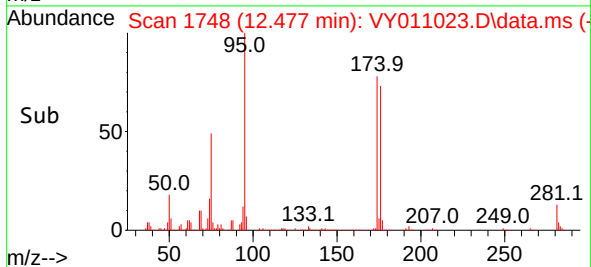
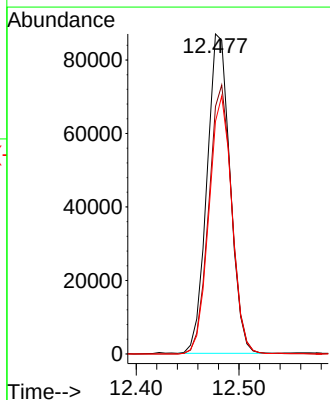
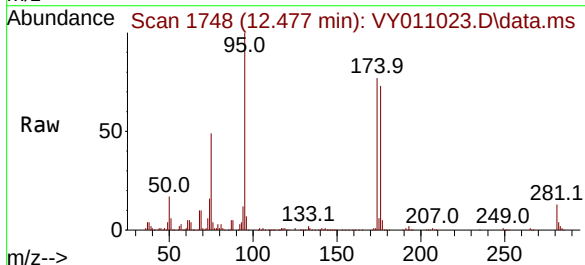


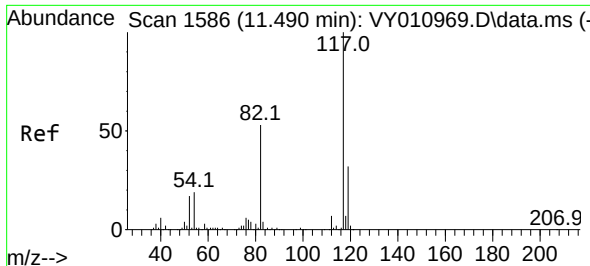

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Instrument :
MSVOA_Y
ClientSampleId :
LSP-SS-02-01-03

Tgt Ion:117 Resp: 345321
Ion Ratio Lower Upper
117 100
82 54.0 43.0 64.4
119 32.0 25.4 38.0

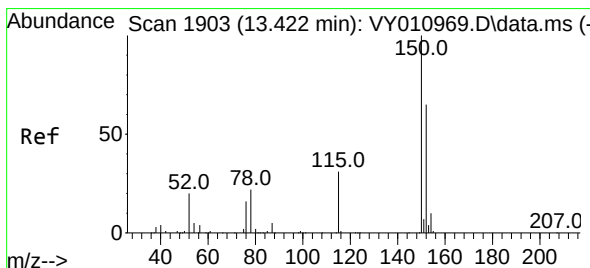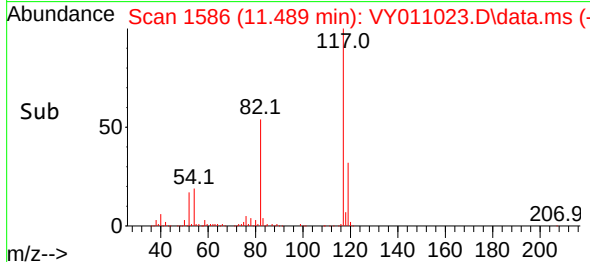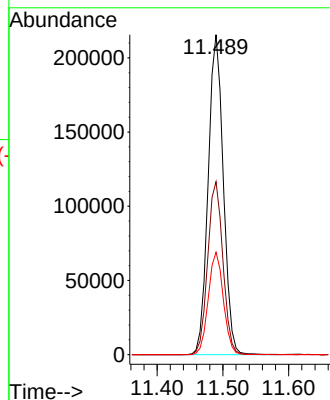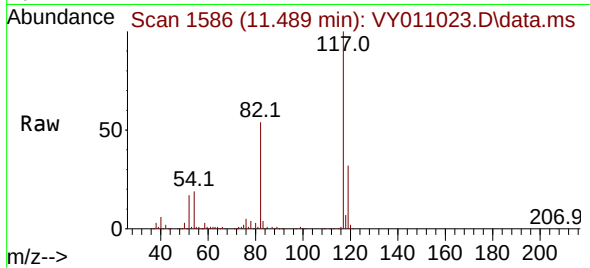

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY011023.D
Acq: 20 Oct 2022 14:27

Tgt Ion:152 Resp: 90638
Ion Ratio Lower Upper
152 100
115 57.5 28.2 84.7
150 157.5 0.0 347.6

