
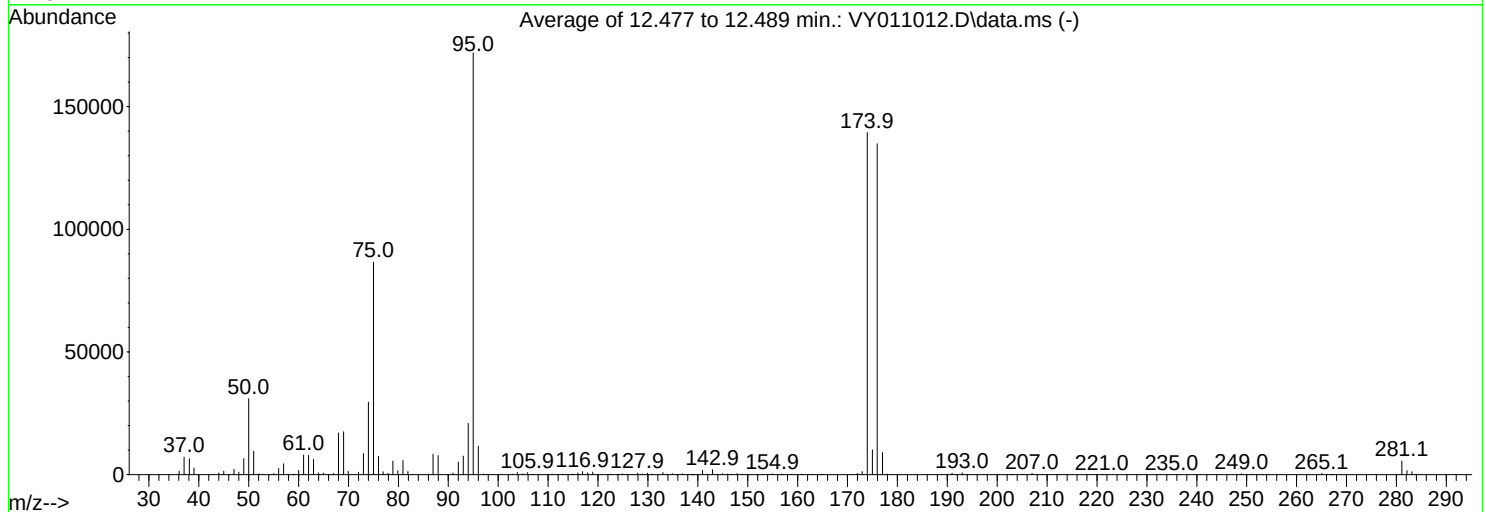


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102022\
 Data File : VY011012.D
 Acq On : 20 Oct 2022 09:17
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
 Title : SW846 8260
 Last Update : Tue Oct 18 01:42:42 2022

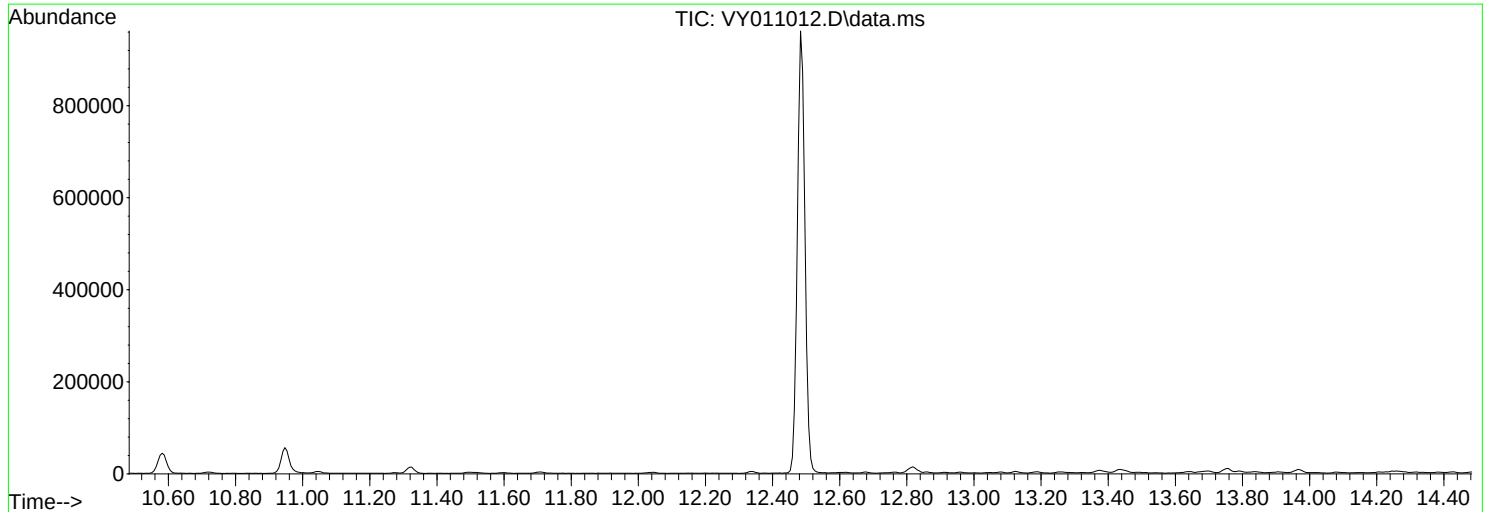

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	30995	PASS
75	95	30	60	50.4	86592	PASS
95	95	100	100	100.0	171925	PASS
96	95	5	9	6.7	11581	PASS
173	174	0.00	2	0.9	1259	PASS
174	95	50	100	81.1	139419	PASS
175	174	5	9	7.3	10128	PASS
176	174	95	101	96.7	134851	PASS
177	176	5	9	6.7	9022	PASS