
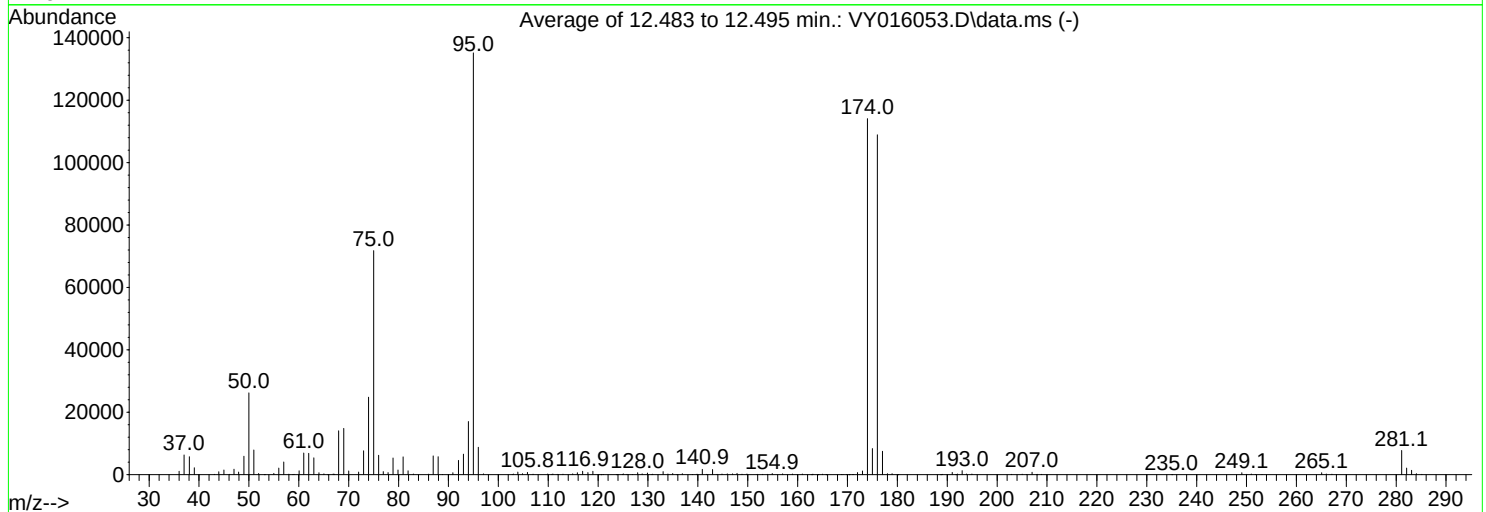


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102023\
Data File : VY016053.D
Acq On : 20 Oct 2023 08:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101823S.M
Title : SW846 8260
Last Update : Thu Oct 19 03:15:44 2023

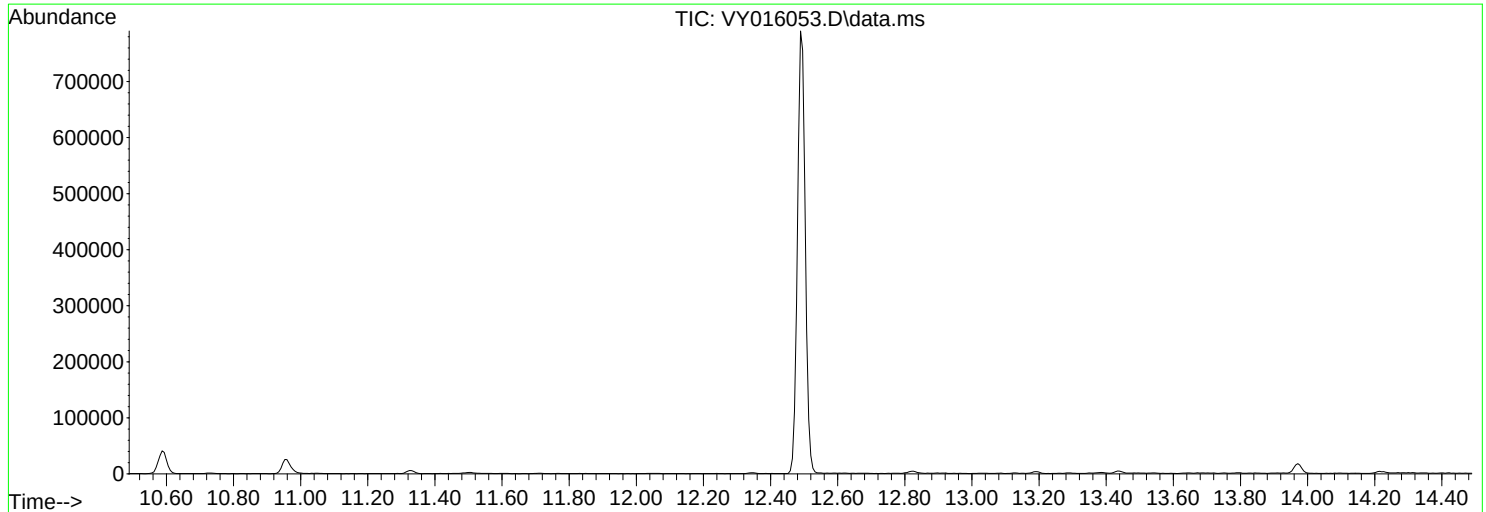

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	26219	PASS
75	95	30	60	53.1	71784	PASS
95	95	100	100	100.0	135165	PASS
96	95	5	9	6.5	8760	PASS
173	174	0.00	2	1.0	1182	PASS
174	95	50	100	84.4	114069	PASS
175	174	5	9	7.3	8350	PASS
176	174	95	101	95.5	108891	PASS
177	176	5	9	6.9	7512	PASS