
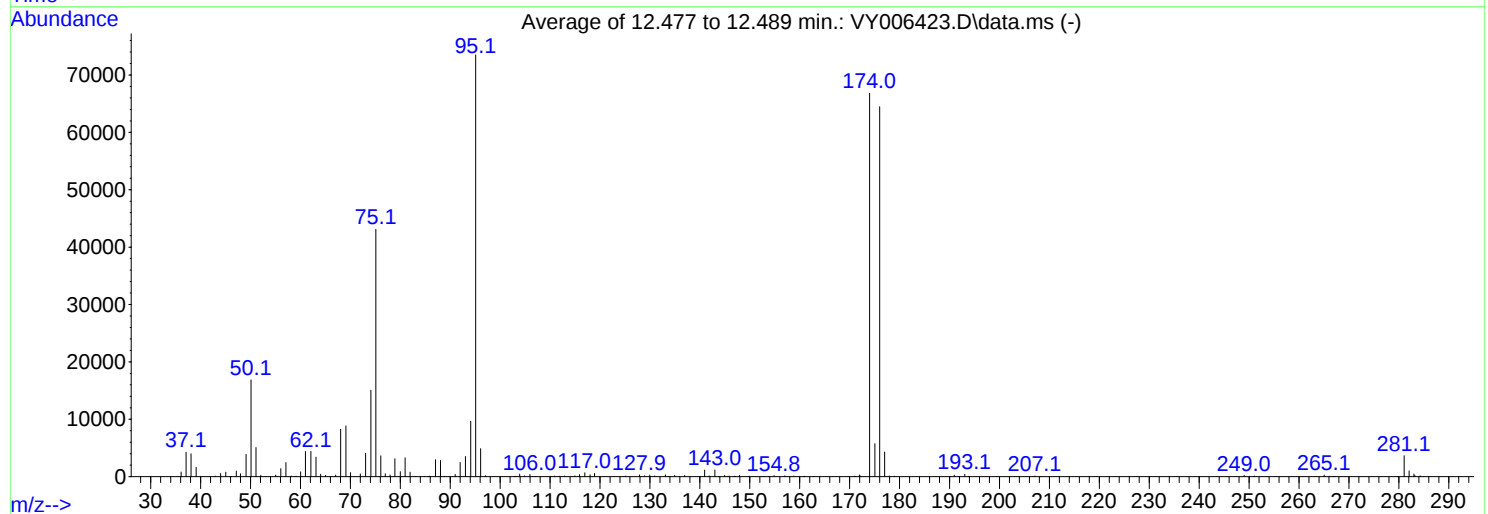


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102121\
Data File : VY006423.D
Acq On : 21 Oct 2021 12:39
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y092821S.M
Title : SW846 8260
Last Update : Tue Sep 28 17:44:36 2021

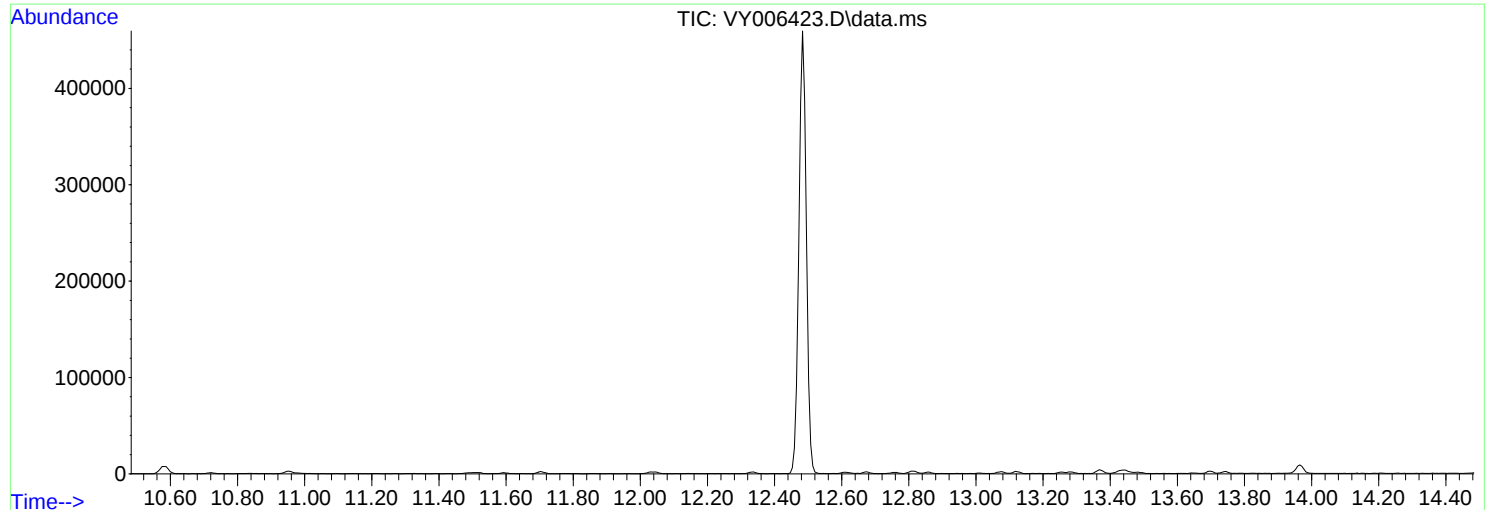

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.9	16867	PASS
75	95	30	60	58.7	43117	PASS
95	95	100	100	100.0	73509	PASS
96	95	5	9	6.6	4884	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.9	66821	PASS
175	174	5	9	8.6	5733	PASS
176	174	95	101	96.5	64469	PASS
177	176	5	9	6.7	4305	PASS