


Methyl Iodide

Response Ratio

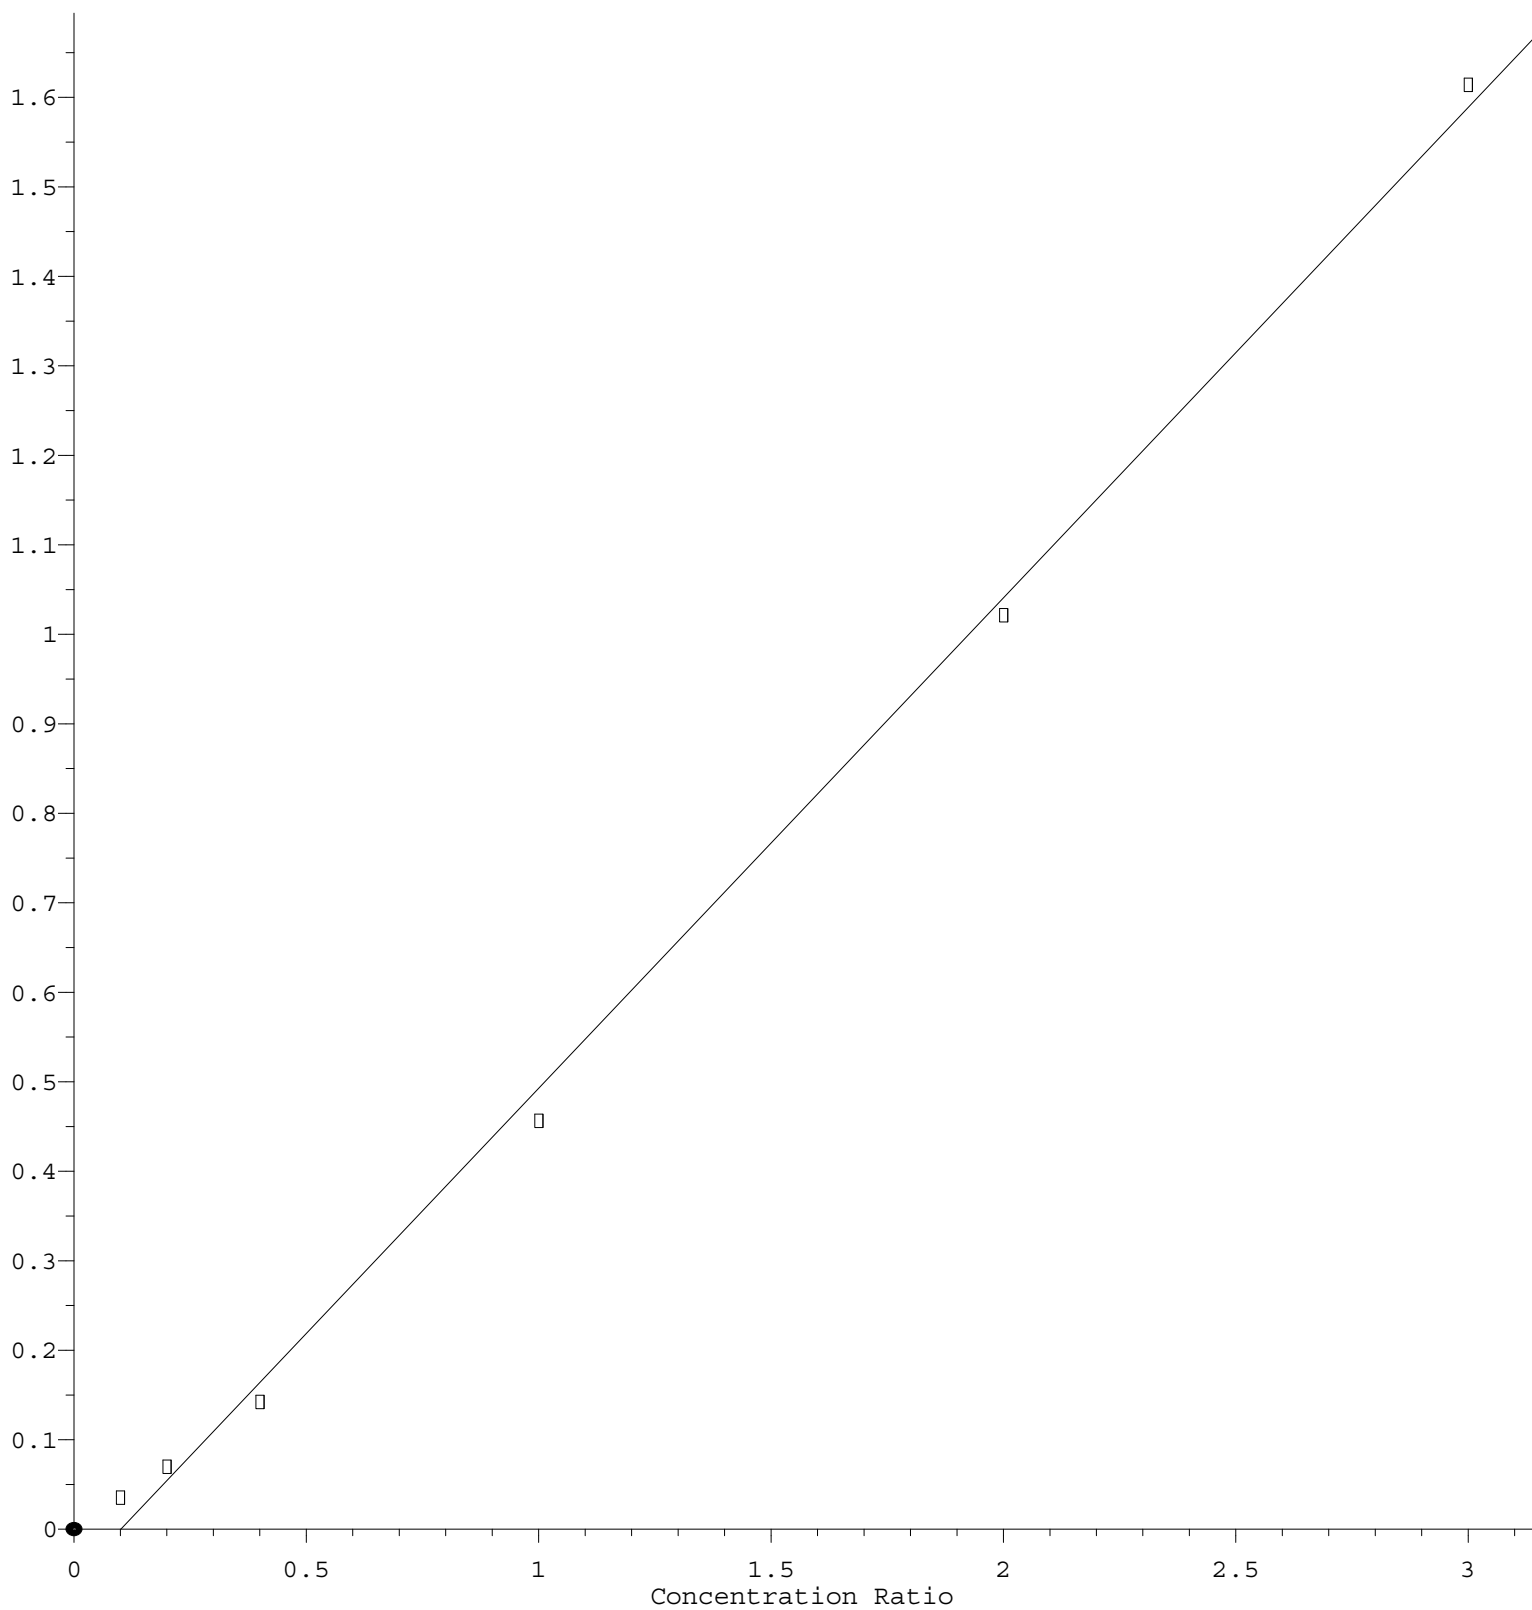

$$\text{Response} = 5.479\text{e-}001 * \text{Amt} - 5.545\text{e-}002$$


Coef of Det (r^2) = 0.997858 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y102221S.M

Calibration Table Last Updated: Sat Oct 23 06:59:04 2021

Methylene Chloride

Response Ratio

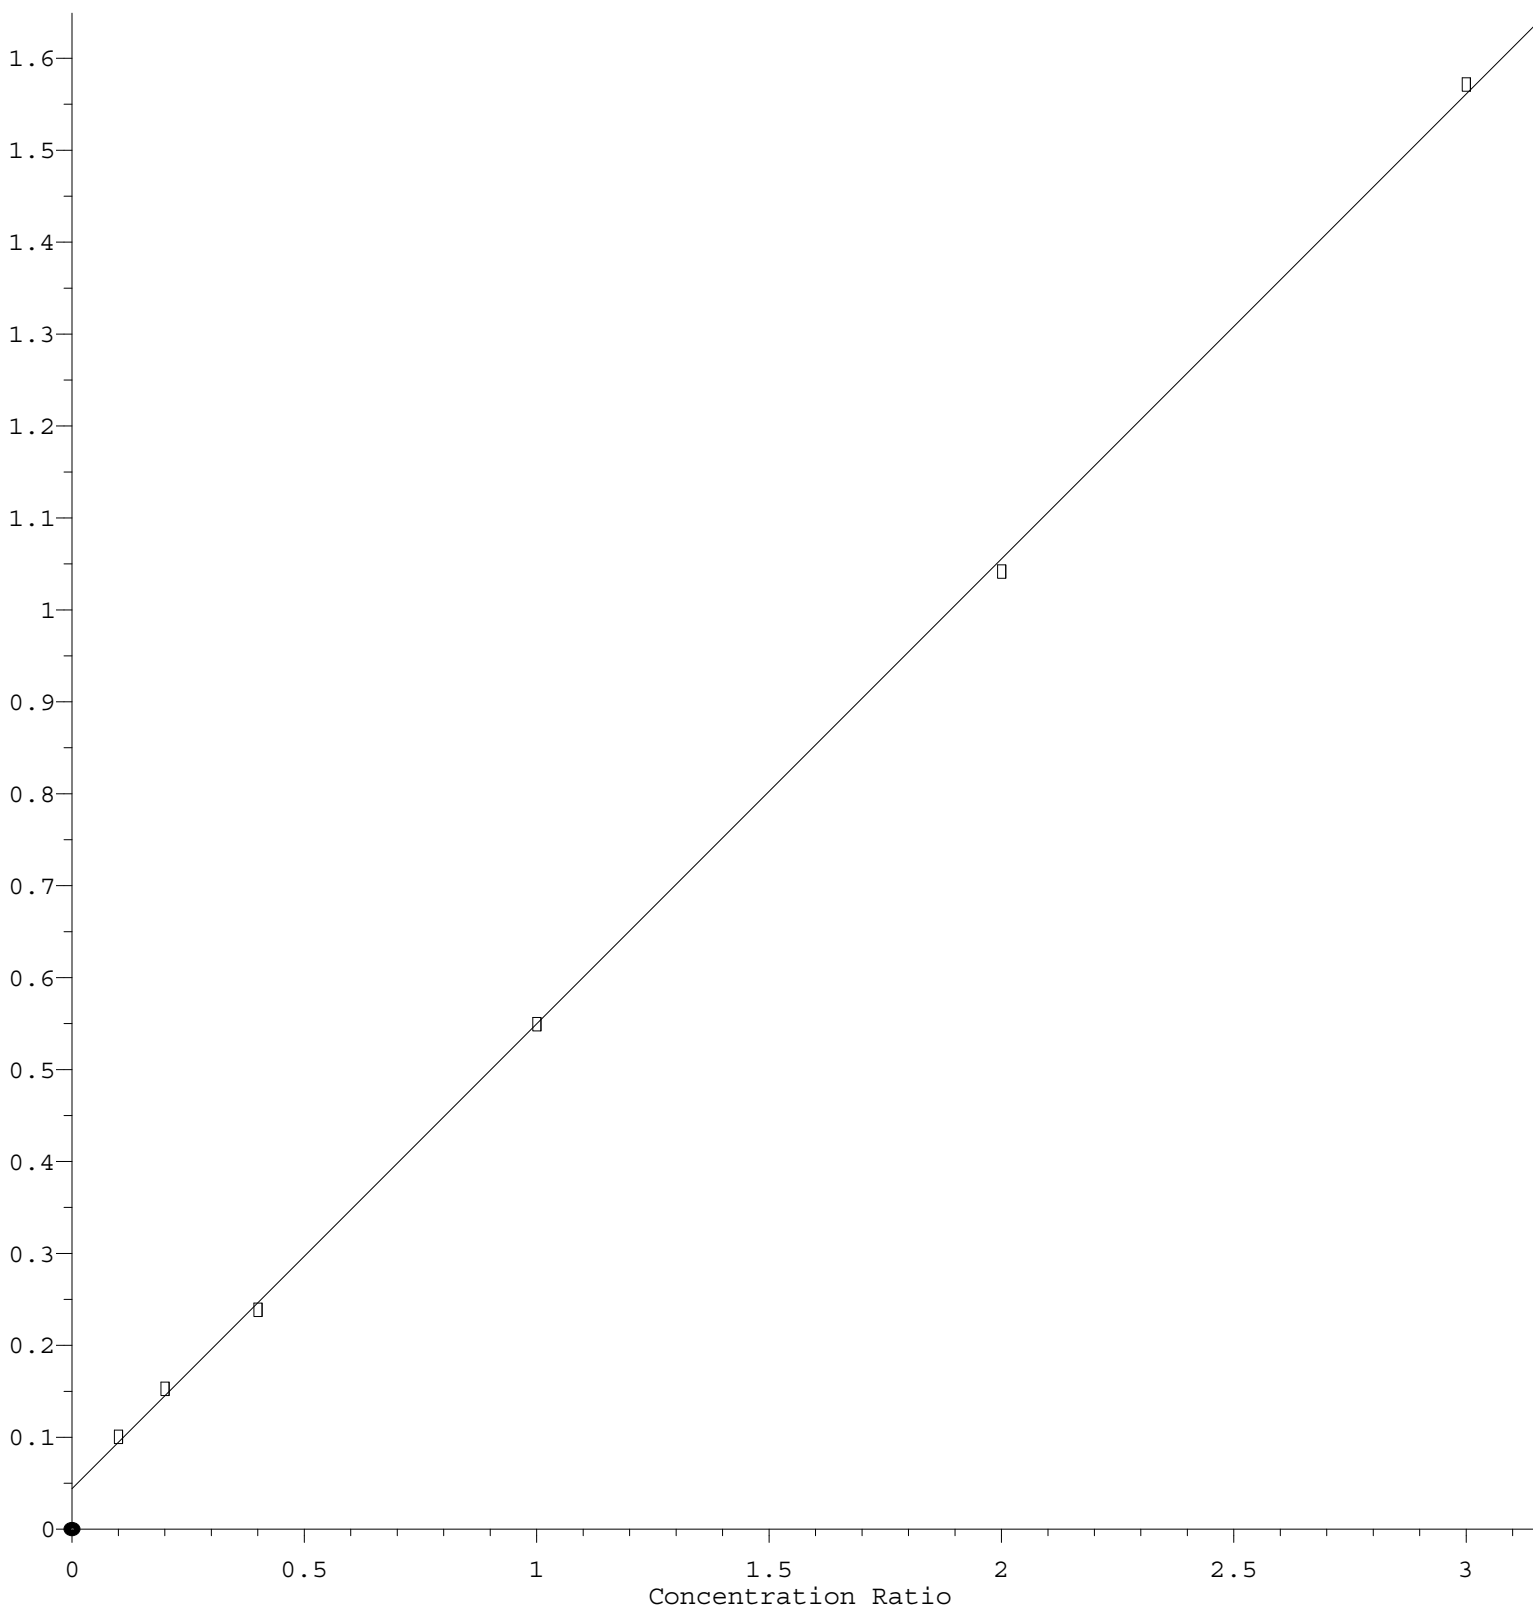

$$\text{Response} = 5.057\text{e-}001 * \text{Amt} + 4.431\text{e-}002$$

Coef of Det (r^2) = 0.999742 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y102221S.M

Calibration Table Last Updated: Sat Oct 23 06:59:04 2021