

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY102319\
 Data File : VY000397.D
 Acq On : 23 Oct 2019 21:23
 Operator : SY/MD
 Sample : K5498-12
 Misc : 4.92G/5ML/MSVOA Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 191-36-(1)

Quant Time: Oct 24 05:30:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 17 02:03:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	210094	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	359545	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	301058	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	112444	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	118311	53.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.78%	
35) Dibromofluoromethane	7.73	113	100942	46.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.08%	
50) Toluene-d8	10.19	98	415424	49.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.58%	
62) 4-Bromofluorobenzene	12.48	95	118870	37.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	75.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY102319\
Data File : VY000397.D
Acq On : 23 Oct 2019 21:23
Operator : SY/MD
Sample : K5498-12
Misc : 4.92G/5ML/MSVOA Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
191-36-(1)

Quant Time: Oct 24 05:30:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 17 02:03:07 2019
Response via : Initial Calibration

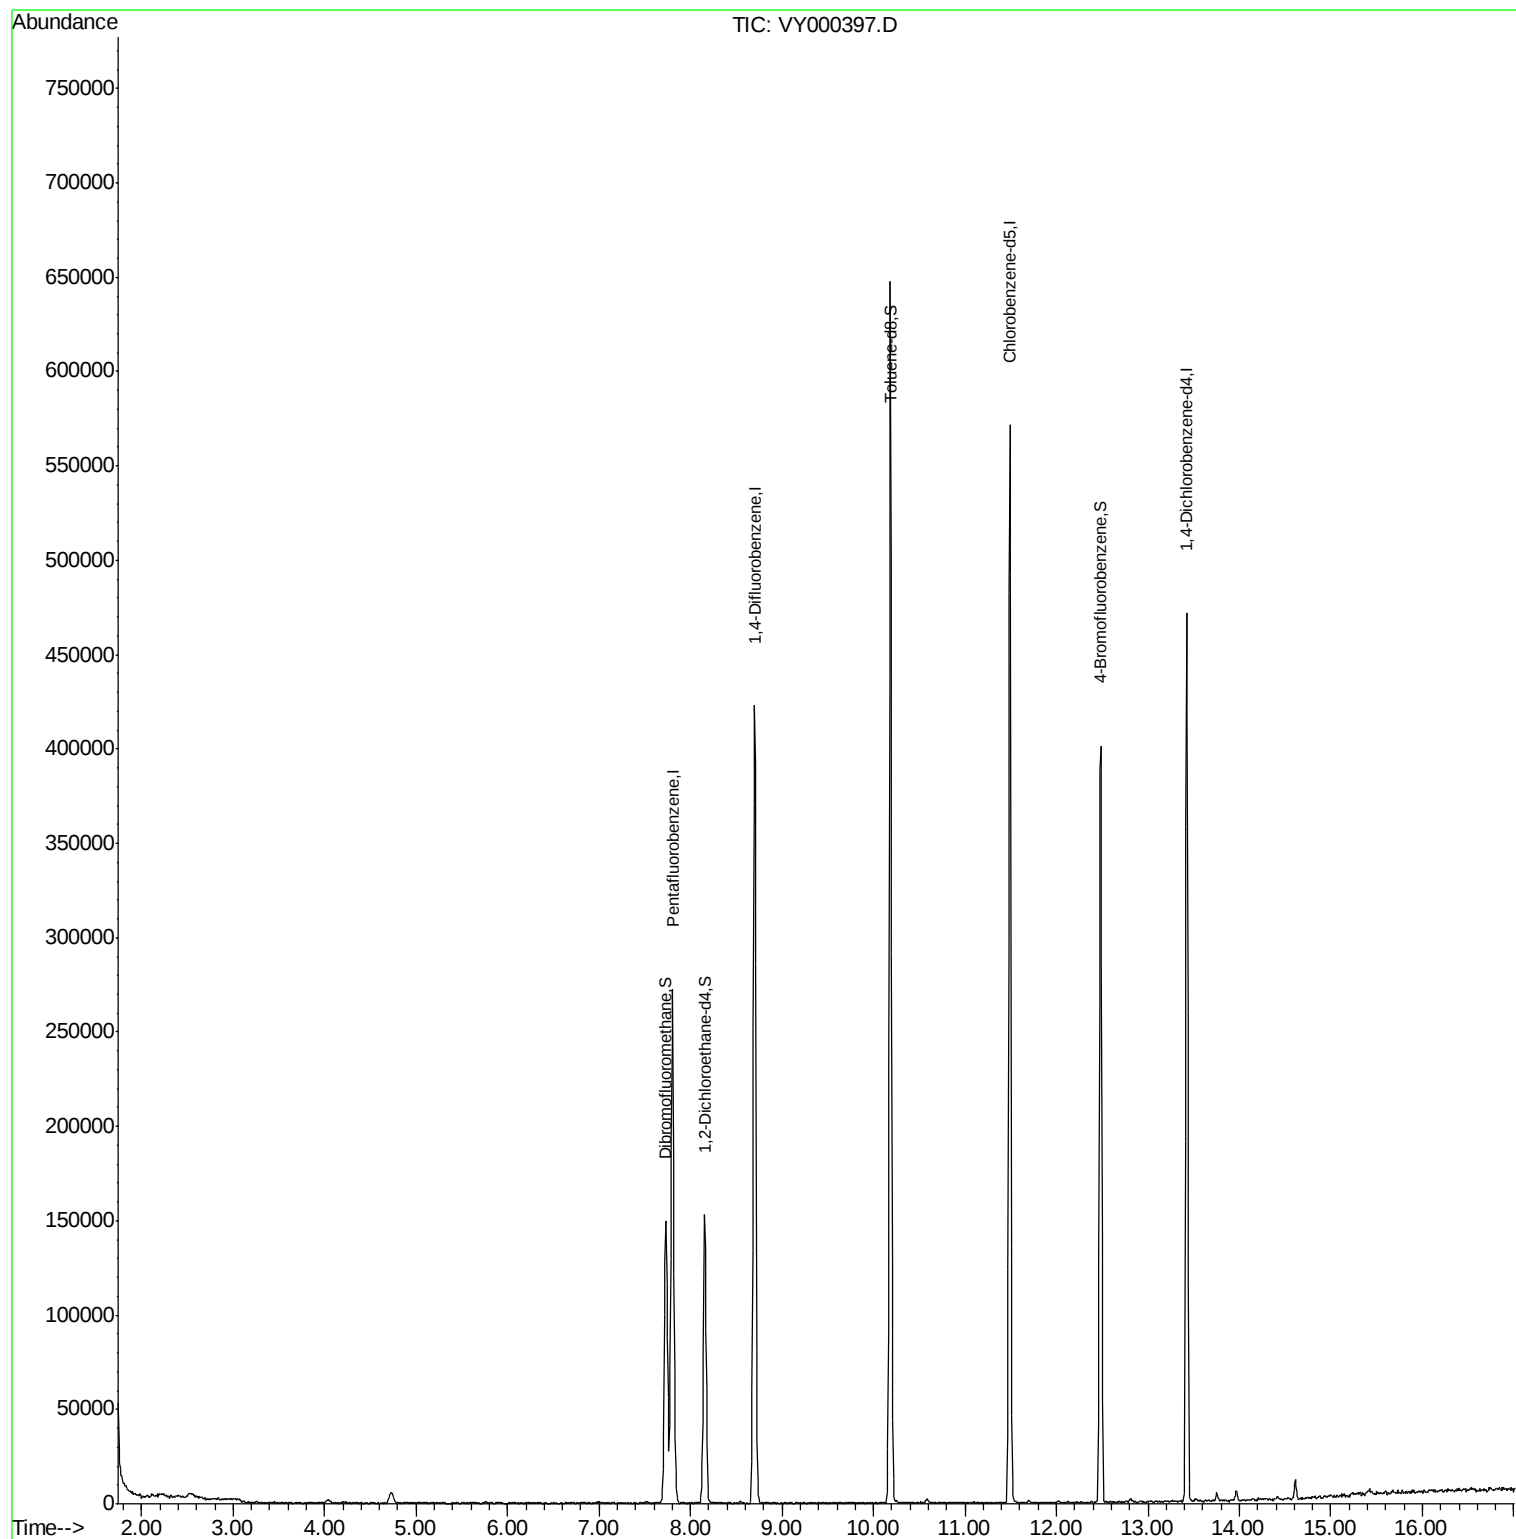

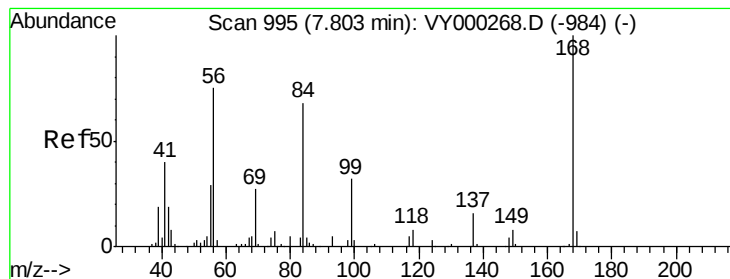

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. -0.00 min

Lab File: VY000397.D

Acq: 23 Oct 2019 21:23

Instrument :

MSVOA_Y

ClientSampleId :


191-36-(1)

Tot Ion:168 Resp: 210094

Ion Ratio Lower Upper

168 100

99 53.1 46.6 69.8

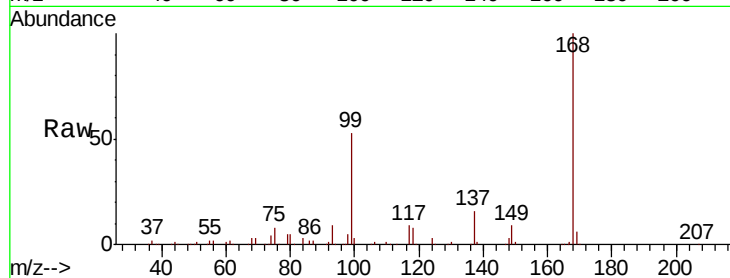

Abundance Ion 167.90 (167.60 to 168.60): VY000397.D (-946) (-)

Ion 98.90 (98.60 to 99.60): VY000397.D (-946) (-)

7.80

100000

80000

60000



40000

20000

0

7.70 7.80 7.90

Time-->

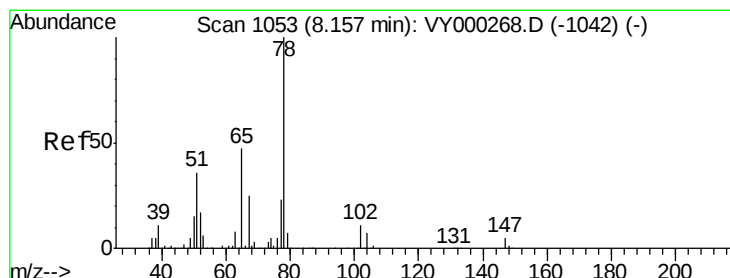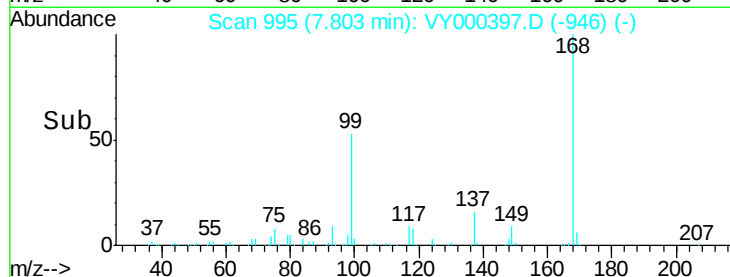

#33

1,2-Dichloroethane-d4

Concen: 53.386 ug/l

RT: 8.16 min Scan# 1053

Delta R.T. -0.00 min

Lab File: VY000397.D


Acq: 23 Oct 2019 21:23

Tgt Ion: 65 Resp: 118311

Ion Ratio Lower Upper

65 100

67 51.4 0.0 109.4

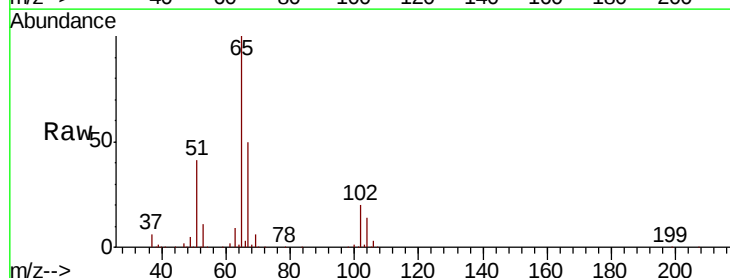

Abundance Ion 64.90 (64.60 to 65.60): VY000397.D (-1004) (-)

Ion 66.90 (66.60 to 67.60): VY000397.D (-1004) (-)

8.16

60000

50000

40000

30000


20000


10000

0

8.10 8.20

Time-->

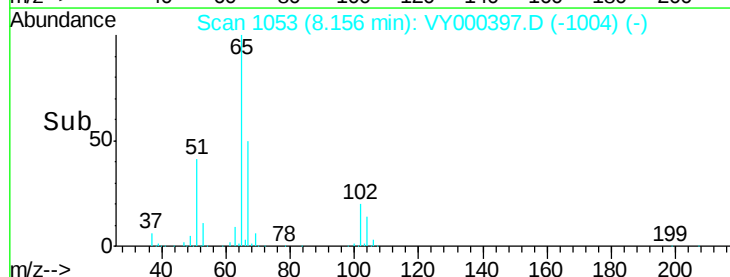

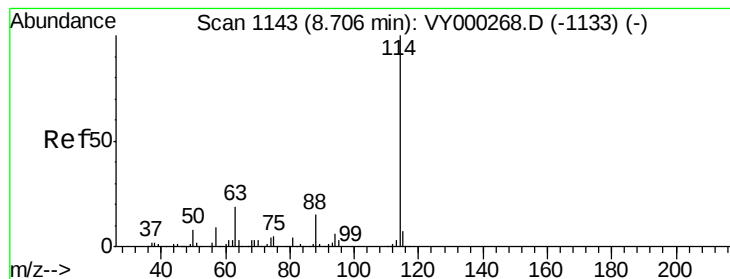

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.70 min Scan# 1142

Delta R.T. -0.01 min

Lab File: VY000397.D

Acq: 23 Oct 2019 21:23

Instrument :

MSVOA_Y

ClientSampleId :

191-36-(1)


Tot Ion:114 Resp: 359545

Ion Ratio Lower Upper

114 100

63 19.4 0.0 37.2




88 13.5 0.0 30.2

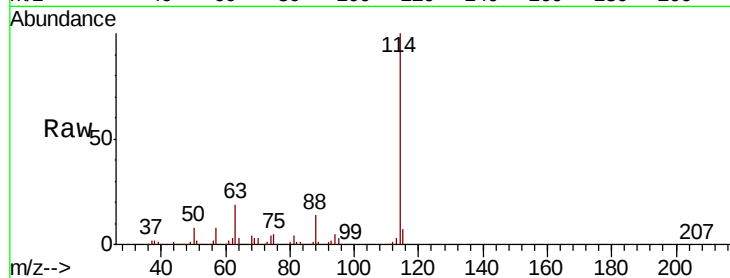

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

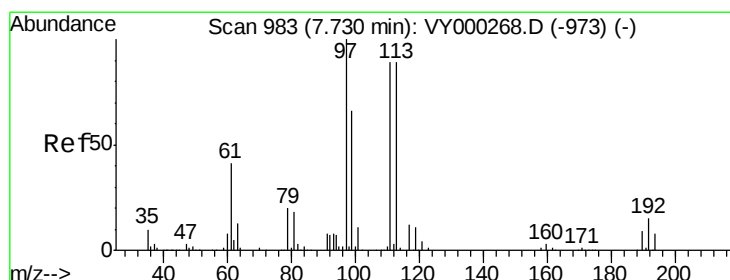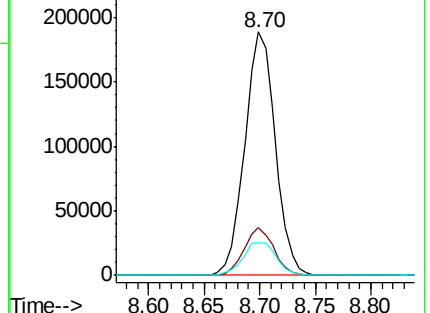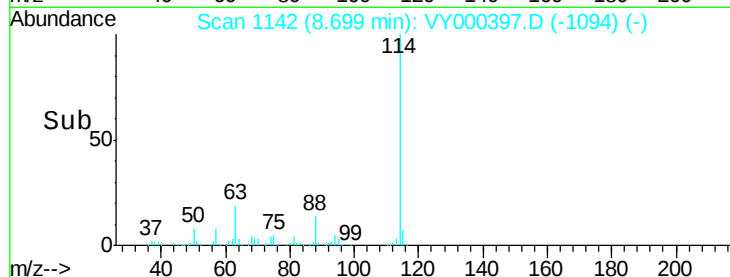

#35

Dibromofluoromethane

Concen: 46.543 ug/l

RT: 7.73 min Scan# 983

Delta R.T. -0.00 min

Lab File: VY000397.D

Acq: 23 Oct 2019 21:23


Tgt Ion:113 Resp: 100942

Ion Ratio Lower Upper

113 100

111 106.1 81.6 122.4



192 20.0 15.3 22.9

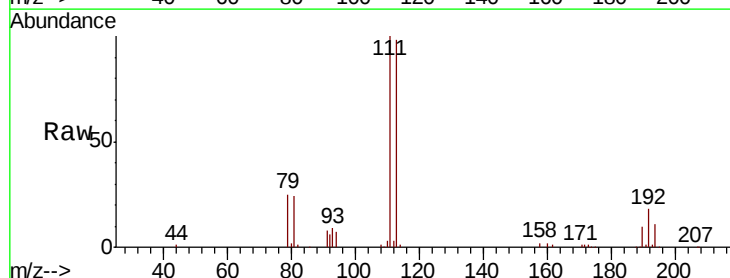


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

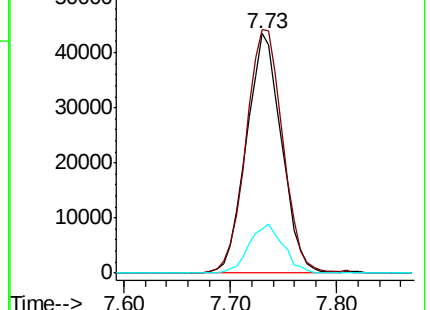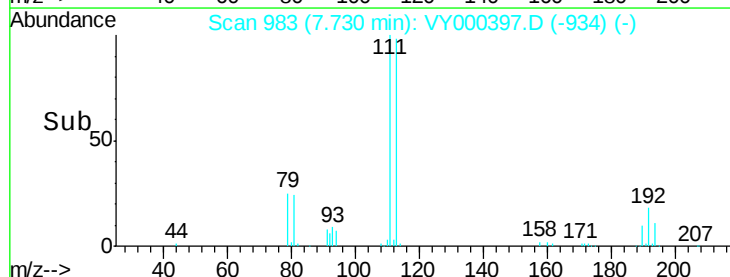

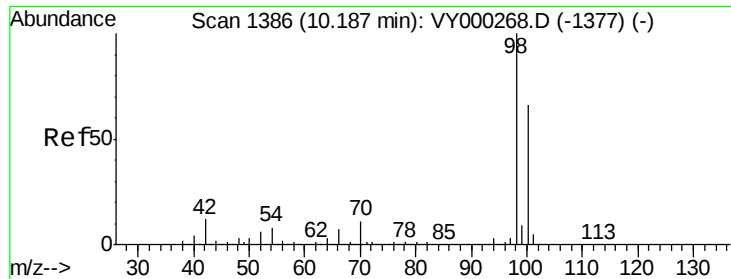

#50

Toluene-d8

Concen: 49.794 ug/l

RT: 10.19 min Scan# 1386

Delta R.T. -0.00 min

Lab File: VY000397.D

Acq: 23 Oct 2019 21:23

Instrument :

MSVOA_Y

ClientSampleId :


191-36-(1)

Tot Ion: 98 Resp: 415424

Ion Ratio Lower Upper




98 100

100 66.8 52.8 79.2

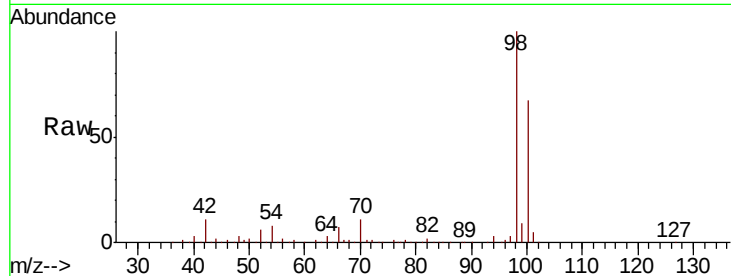

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

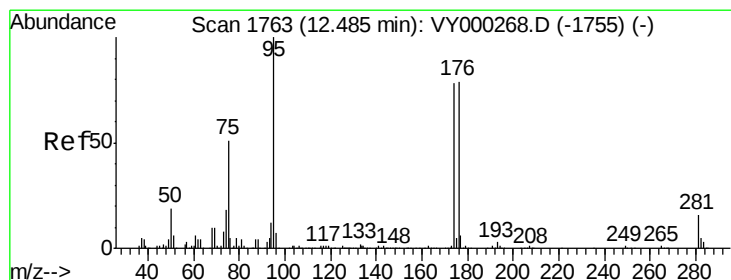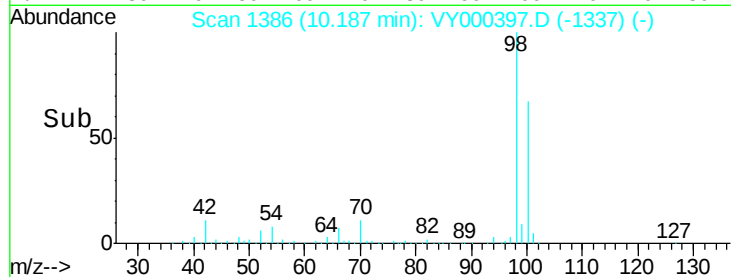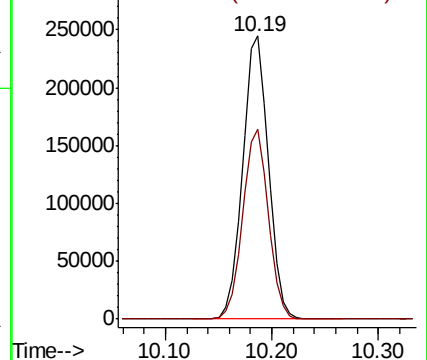

#62

4-Bromofluorobenzene

Concen: 37.504 ug/l

RT: 12.48 min Scan# 1763

Delta R.T. -0.00 min

Lab File: VY000397.D

Acq: 23 Oct 2019 21:23


Tgt Ion: 95 Resp: 118870

Ion Ratio Lower Upper

95 100

174 84.1 0.0 159.6



176 81.5 0.0 153.8

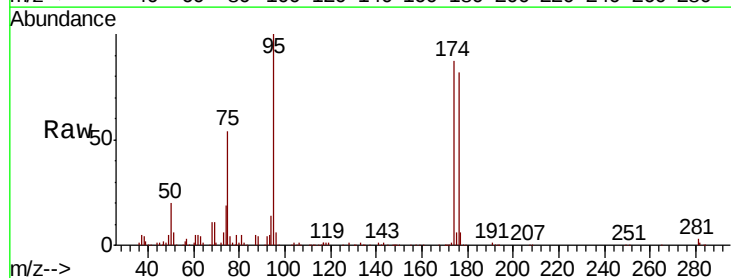


Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



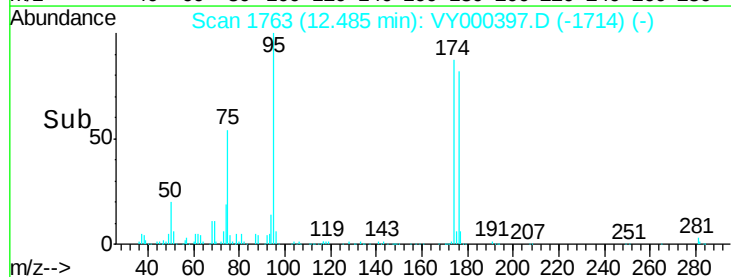
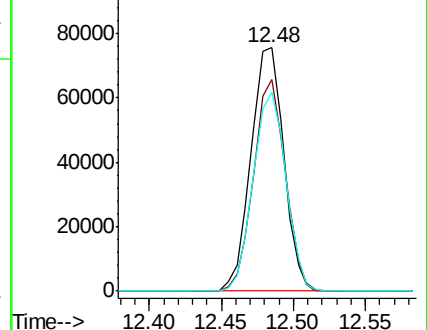


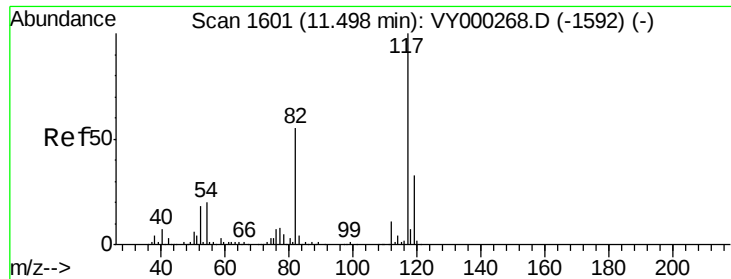

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.01 min
Lab File: VY000397.D
Acq: 23 Oct 2019 21:23

Instrument :
MSVOA_Y
ClientSampled :
191-36-(1)

Tot Ion	Ratio	Lower	Upper
117	100		
82	54.7	43.7	65.5
119	31.4	26.6	39.8

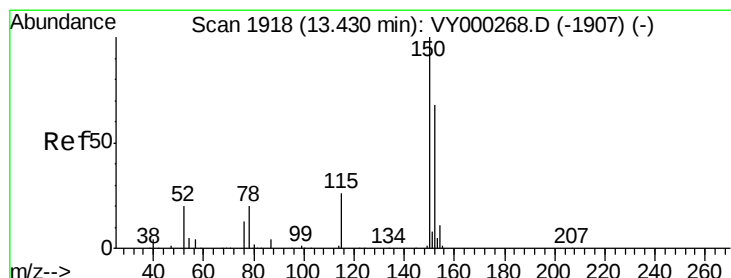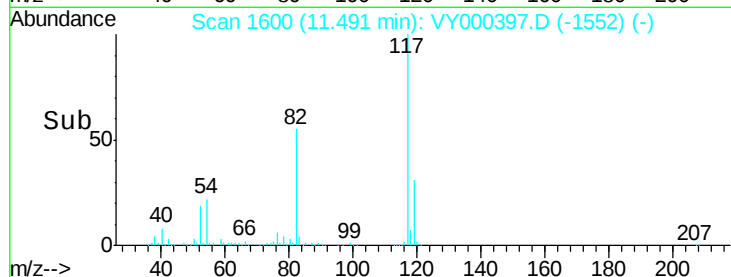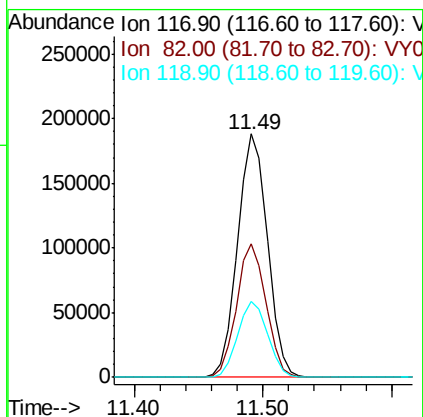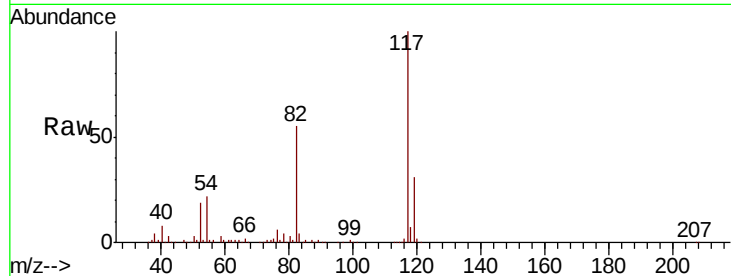

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.01 min
Lab File: VY000397.D
Acq: 23 Oct 2019 21:23

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.6	29.3	88.0
150	158.2	0.0	348.4

