

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY102519\
 Data File : VY000442.D
 Acq On : 25 Oct 2019 20:20
 Operator : SY/MD
 Sample : K5540-12
 Misc : 5.08G/5ML/MSVOA Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 157-72-(1.1)

Quant Time: Oct 26 03:15:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 17 02:03:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	182239	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	312906	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	275490	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	106021	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	107732	56.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.08%	
35) Dibromofluoromethane	7.74	113	92504	49.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.02%	
50) Toluene-d8	10.19	98	359264	49.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.96%	
62) 4-Bromofluorobenzene	12.48	95	110297	39.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	79.98%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY102519\
Data File : VY000442.D
Acq On : 25 Oct 2019 20:20
Operator : SY/MD
Sample : K5540-12
Misc : 5.08G/5ML/MSVOA Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
157-72-(1.1)

Quant Time: Oct 26 03:15:44 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 17 02:03:07 2019
Response via : Initial Calibration

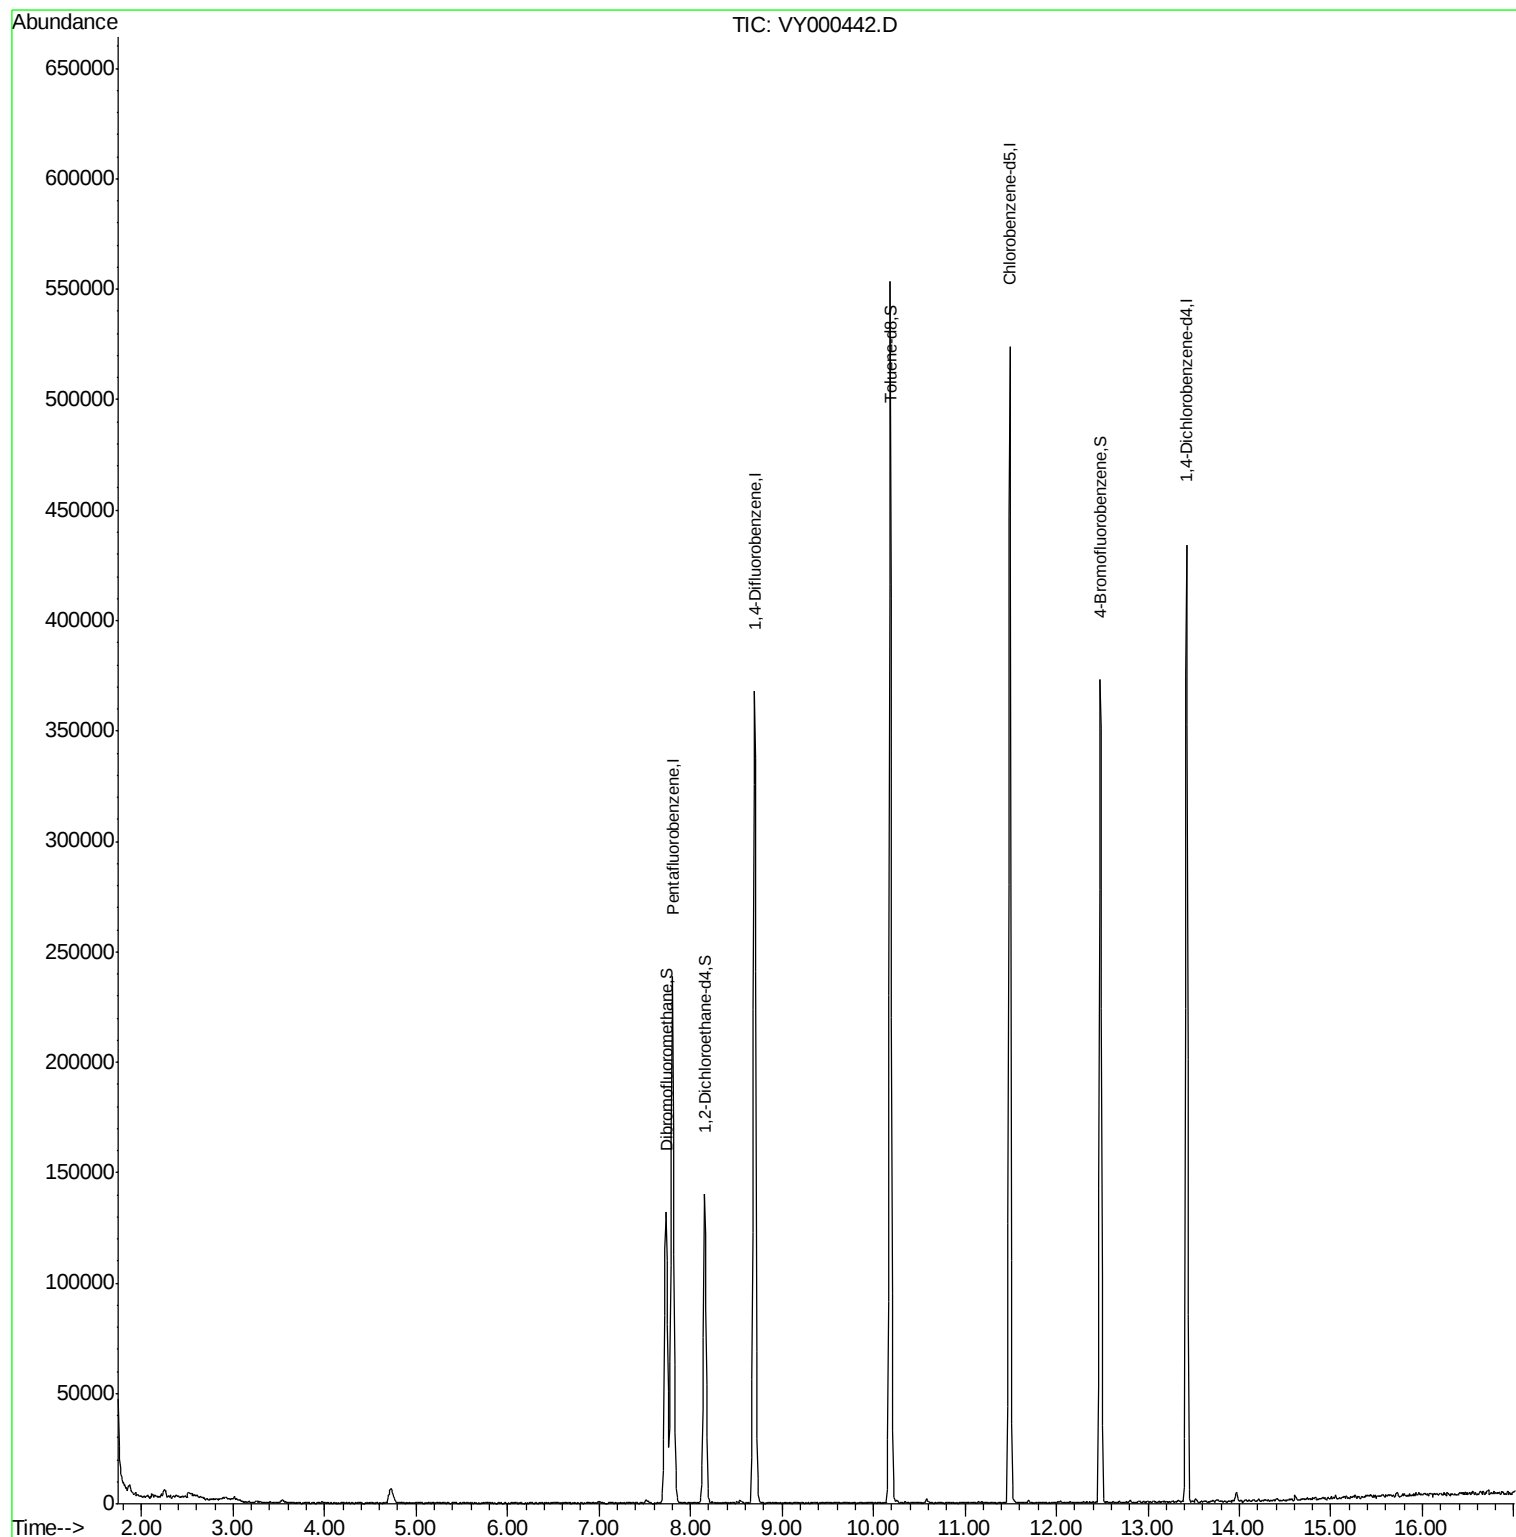


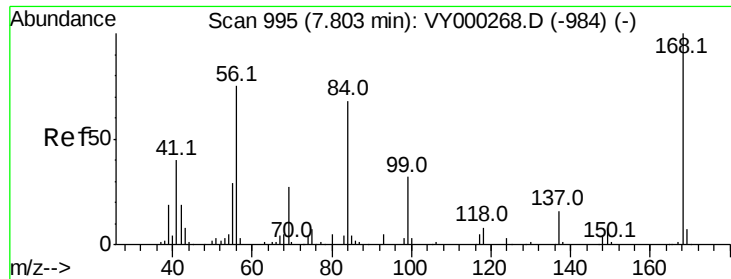




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.80 min Scan# 995
Delta R.T. -0.00 min
Lab File: VY000442.D
Acq: 25 Oct 2019 20:20

Instrument :
MSVOA_Y
ClientSampleId :
157-72-(1.1)

Tot Ion:168 Resp: 182239
Ion Ratio Lower Upper
168 100
99 56.9 46.6 69.8

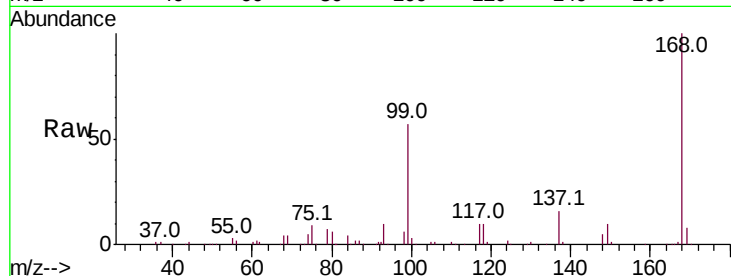


Abundance Ion 167.90 (167.60 to 168.60): VY000442.D (-1042) (-)
Ion 98.90 (98.60 to 99.60): VY000442.D (-1042) (-)

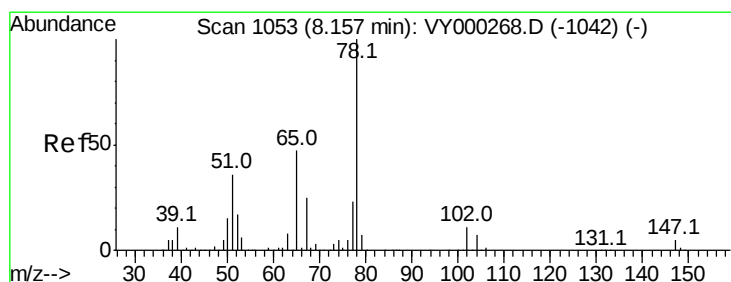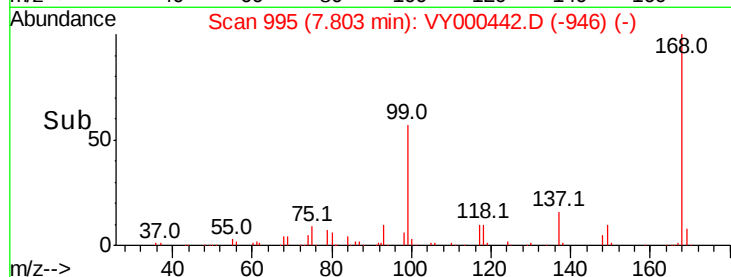
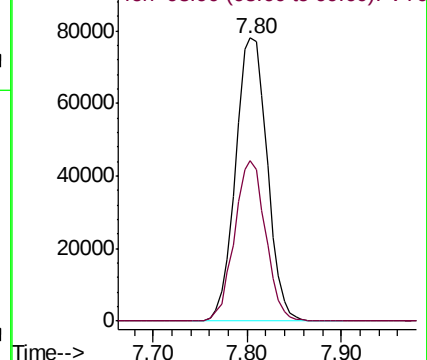



#33
1,2-Dichloroethane-d4
Concen: 56.042 ug/l
RT: 8.16 min Scan# 1053
Delta R.T. -0.00 min
Lab File: VY000442.D
Acq: 25 Oct 2019 20:20

Tgt Ion: 65 Resp: 107732
Ion Ratio Lower Upper
65 100
67 53.0 0.0 109.4

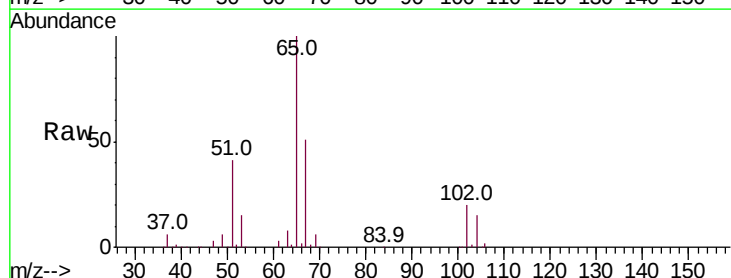

Abundance Ion 64.90 (64.60 to 65.60): VY000442.D (-1004) (-)
Ion 66.90 (66.60 to 67.60): VY000442.D (-1004) (-)

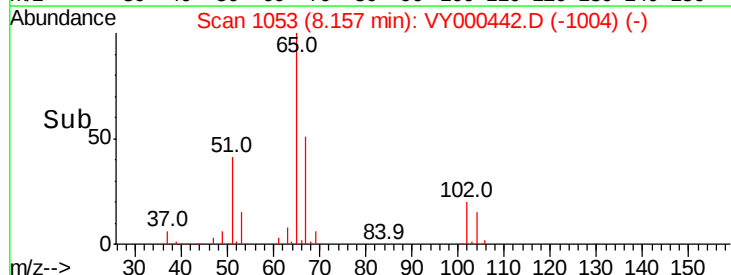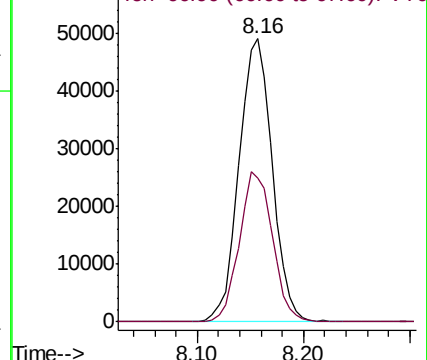


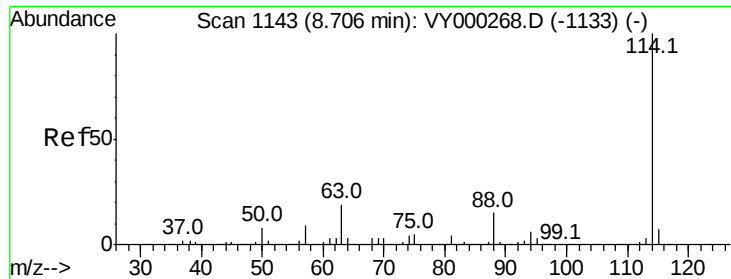




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.70 min Scan# 1142
 Delta R.T. -0.01 min
 Lab File: VY000442.D
 Acq: 25 Oct 2019 20:20

Instrument :
 MSVOA_Y
 ClientSampleId :
 157-72-(1.1)

Tot Ion:	114	Resp:	312906
Ion	Ratio	Lower	Upper
114	100		
63	19.0	0.0	37.2
88	14.6	0.0	30.2

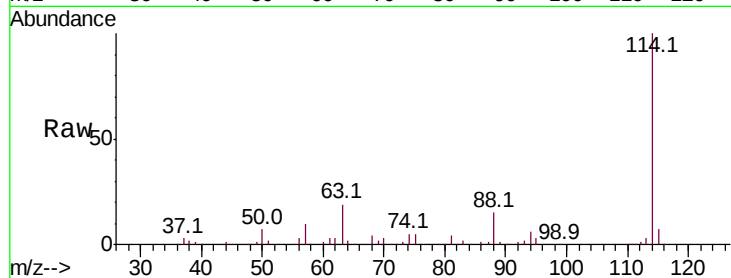


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VY0
 Ion 87.90 (87.60 to 88.60): VY0

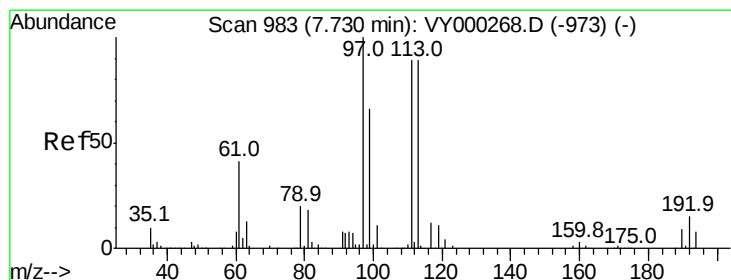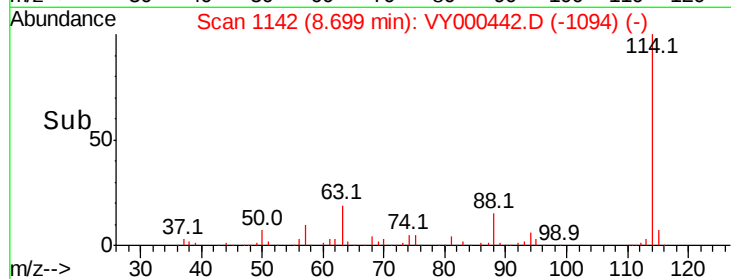
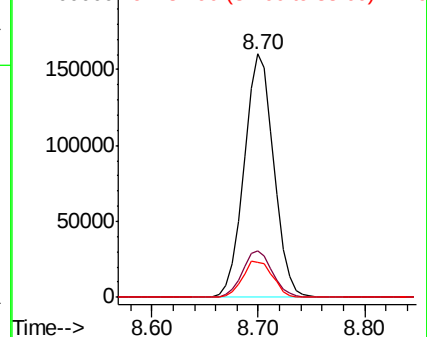



#35
 Dibromofluoromethane
 Concen: 49.009 ug/l
 RT: 7.74 min Scan# 984
 Delta R.T. 0.01 min
 Lab File: VY000442.D
 Acq: 25 Oct 2019 20:20

Tgt Ion:	113	Resp:	92504
Ion	Ratio	Lower	Upper
113	100		
111	101.4	81.6	122.4
192	19.4	15.3	22.9

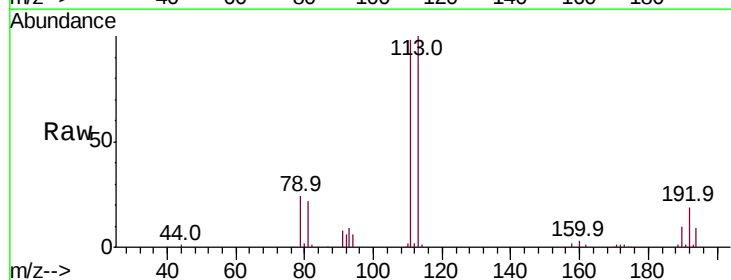

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

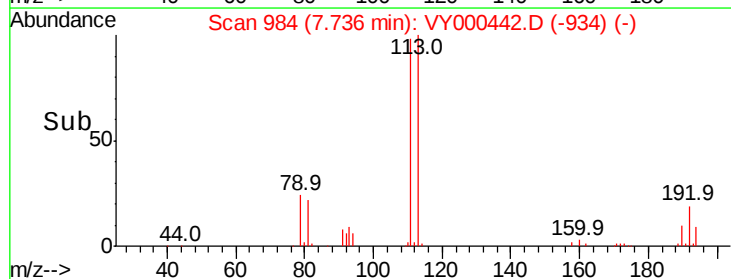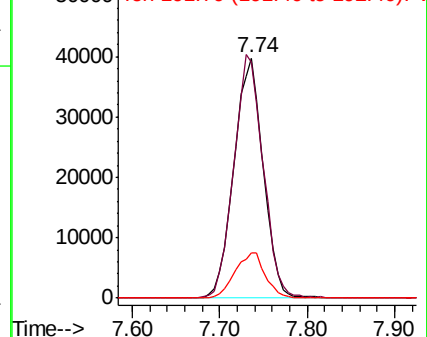

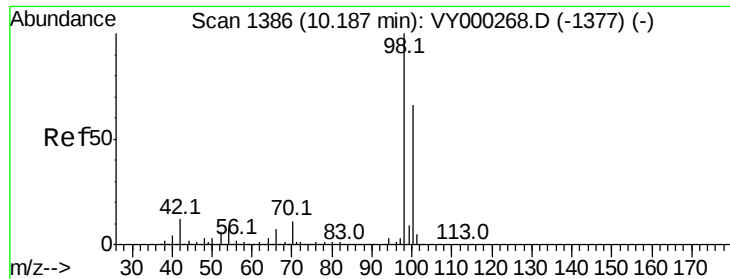

#50

Toluene-d8

Concen: 49.481 ug/l

RT: 10.19 min Scan# 1386

Delta R.T. -0.00 min

Lab File: VY000442.D

Acq: 25 Oct 2019 20:20

Instrument :

MSVOA_Y

ClientSampleId :


157-72-(1.1)

Tot Ion: 98 Resp: 359264

Ion Ratio Lower Upper

98 100

100 66.1 52.8 79.2

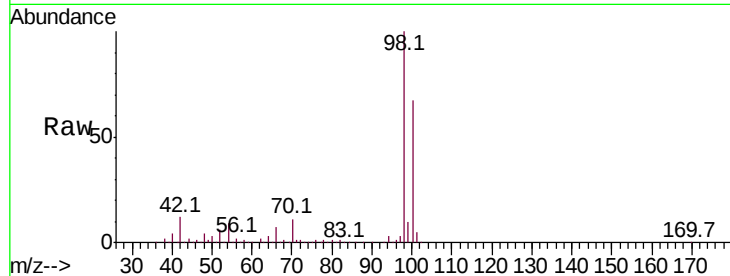

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

200000

150000



100000

50000

0

10.10 10.20 10.30

Time-->

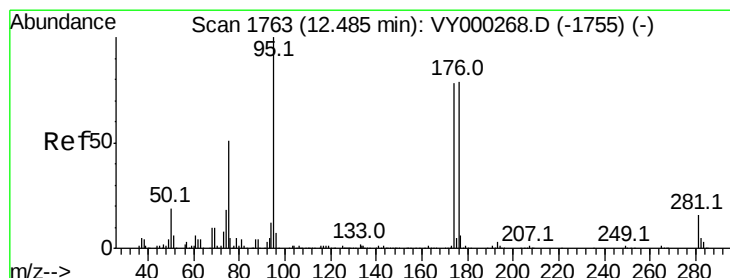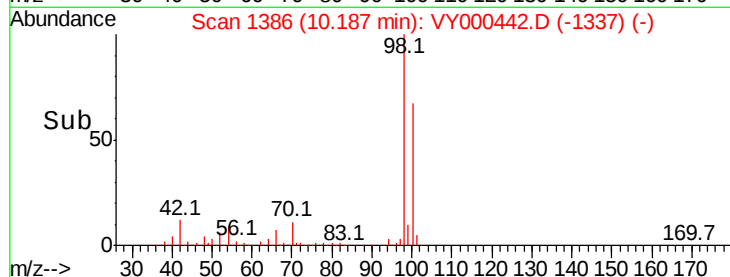

#62

4-Bromofluorobenzene

Concen: 39.986 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.01 min

Lab File: VY000442.D

Acq: 25 Oct 2019 20:20


Tgt Ion: 95 Resp: 110297

Ion Ratio Lower Upper

95 100

174 82.4 0.0 159.6

176 82.0 0.0 153.8

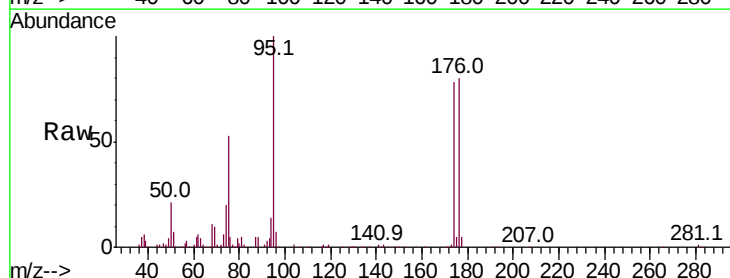

Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

100000

80000

60000


40000


20000

0

12.40 12.45 12.50 12.55

Time-->

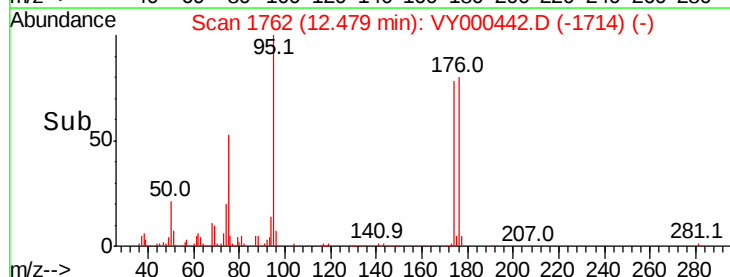


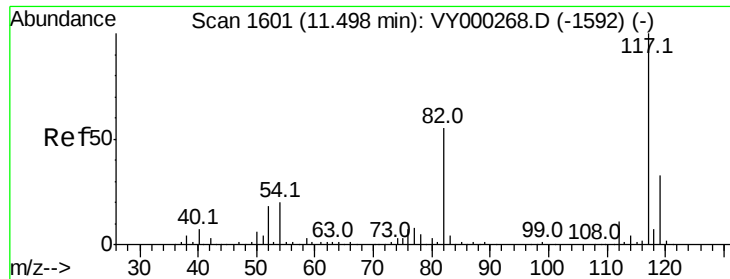




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.01 min
Lab File: VY000442.D
Acq: 25 Oct 2019 20:20

Instrument :
MSVOA_Y
ClientSampleId :
157-72-(1.1)

Tot Ion:117 Resp: 275490
Ion Ratio Lower Upper
117 100
82 51.5 43.7 65.5
119 31.8 26.6 39.8

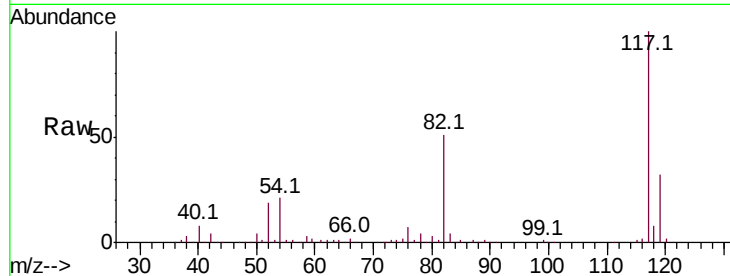


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

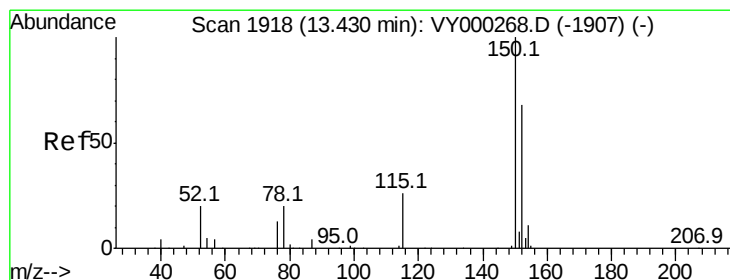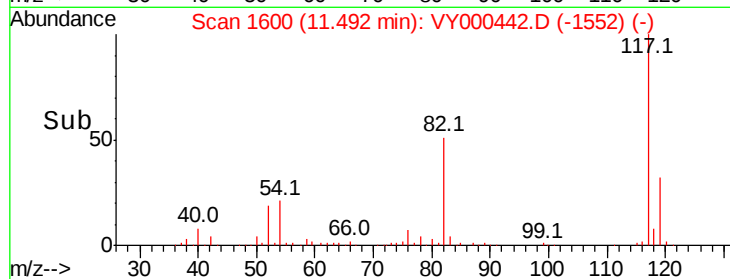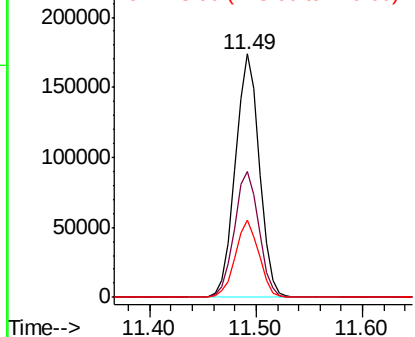

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.01 min
Lab File: VY000442.D
Acq: 25 Oct 2019 20:20

Tgt Ion:152 Resp: 106021
Ion Ratio Lower Upper
152 100
115 56.6 29.3 88.0
150 158.0 0.0 348.4

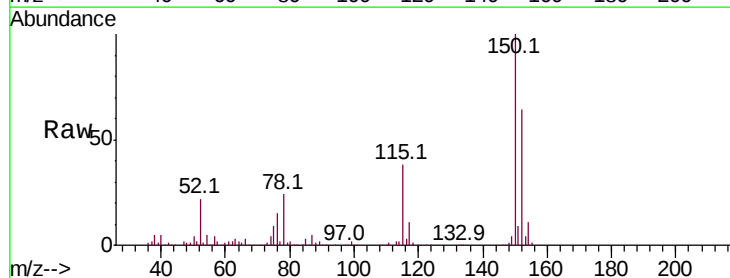

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

