

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102621\
 Data File : VY006481.D
 Acq On : 26 Oct 2021 15:13
 Operator : SY/MD
 Sample : M4329-01
 Misc : 3.29G/5ML/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PSC124019

Quant Time: Oct 27 05:26:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 23 06:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	102214	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	170414	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	160016	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	69911	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	74181	58.976	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	117.960%
35) Dibromofluoromethane	7.722	113	51639	54.366	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.740%
50) Toluene-d8	10.185	98	222231	55.192	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	110.380%
62) 4-Bromofluorobenzene	12.483	95	72368	53.354	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	106.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102621\
Data File : VY006481.D
Acq On : 26 Oct 2021 15:13
Operator : SY/MD
Sample : M4329-01
Misc : 3.29G/5ML/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PSC124019

Quant Time: Oct 27 05:26:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
Quant Title : SW846 8260
QLast Update : Sat Oct 23 06:59:04 2021
Response via : Initial Calibration




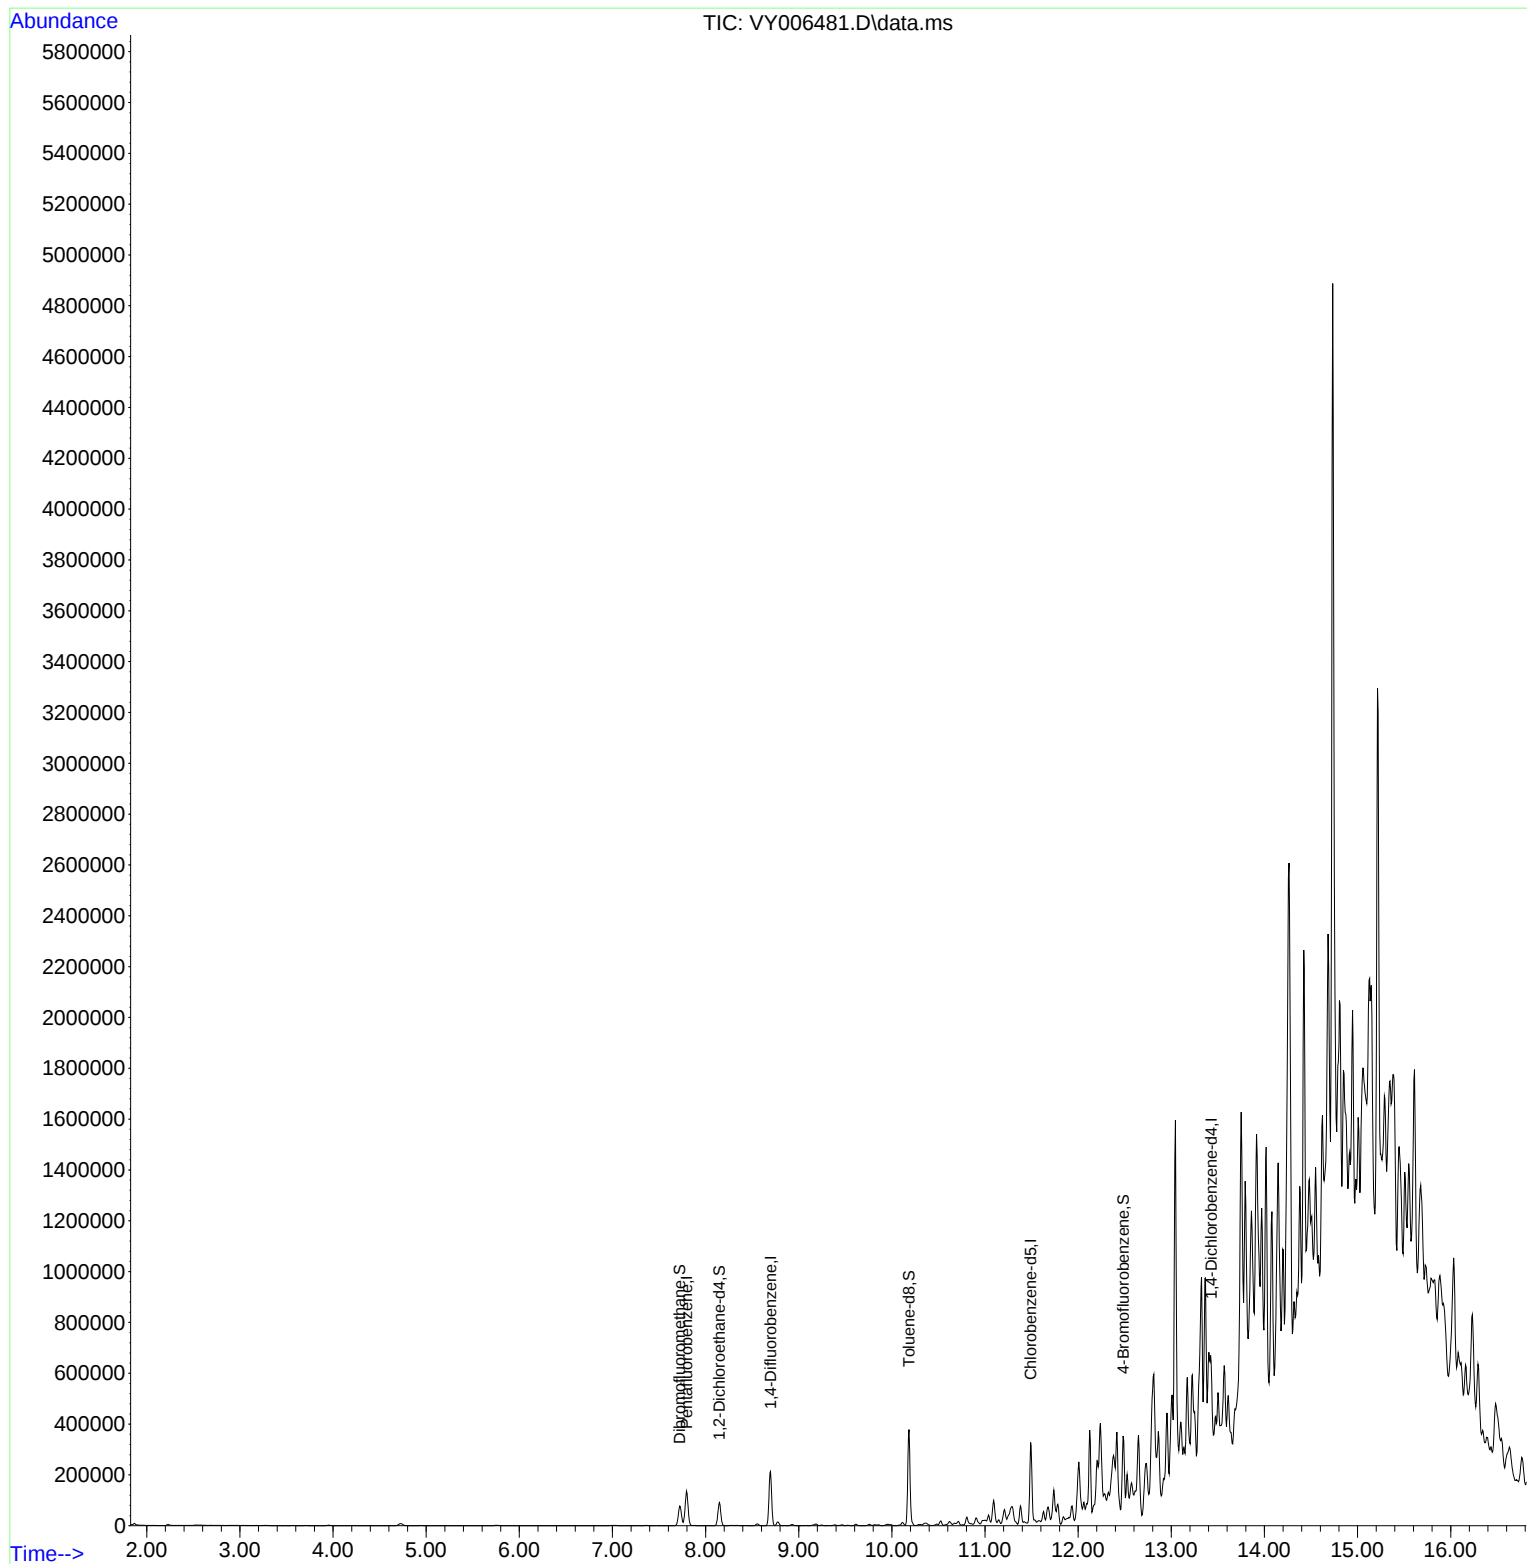


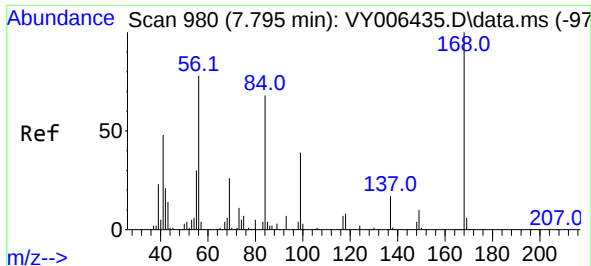

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13




Instrument :
MSVOA_Y
ClientSampleId :
PSC124019


Tgt Ion:168 Resp: 102214
Ion Ratio Lower Upper
168 100
99 57.1 44.8 67.2

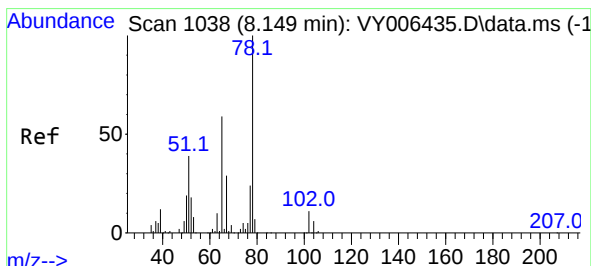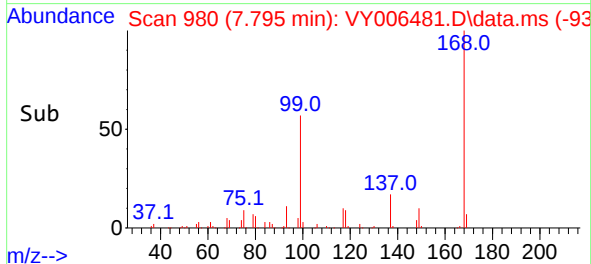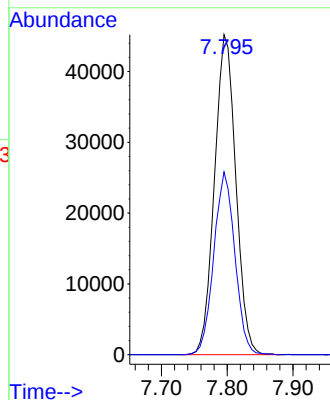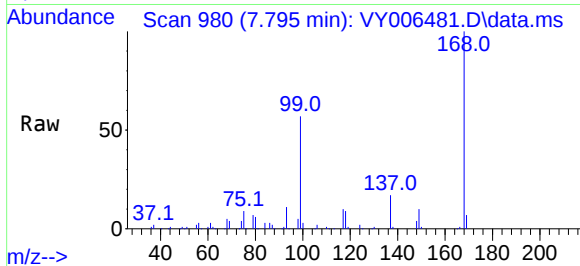

#33
1,2-Dichloroethane-d4
Concen: 58.976 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13

Tgt Ion: 65 Resp: 74181
Ion Ratio Lower Upper
65 100
67 49.9 0.0 98.2

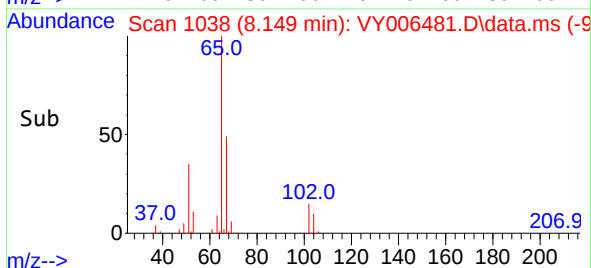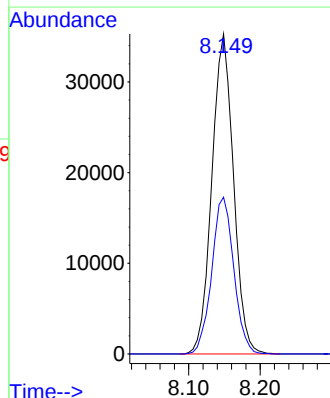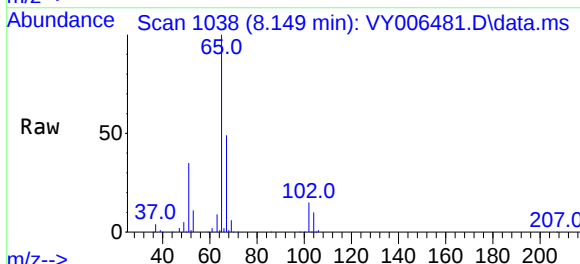

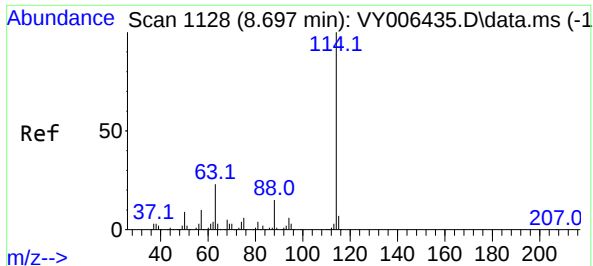

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. 0.000 min

Lab File: VY006481.D

Acq: 26 Oct 2021 15:13

Instrument :

MSVOA_Y

ClientSampleId :

PSC124019





Tgt Ion:114 Resp: 170414

Ion Ratio Lower Upper

114 100

63 22.0 0.0 45.0

88 15.2 0.0 30.6

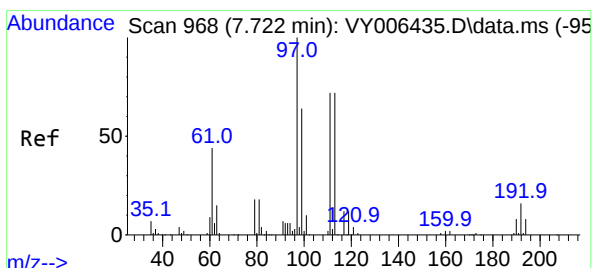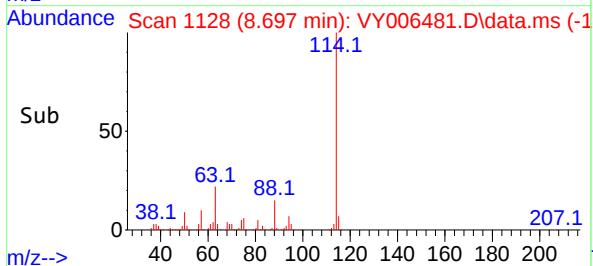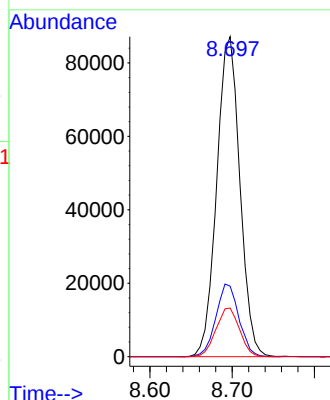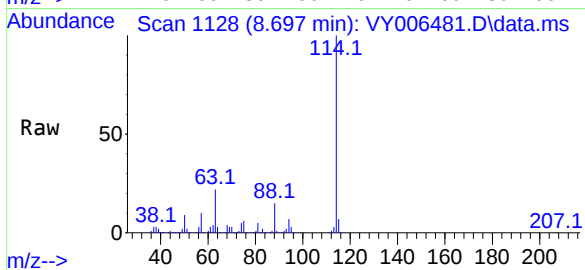

#35

Dibromofluoromethane

Concen: 54.366 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.000 min

Lab File: VY006481.D

Acq: 26 Oct 2021 15:13




Tgt Ion:113 Resp: 51639


Ion Ratio Lower Upper

113 100

111 101.9 82.3 123.5

192 22.1 17.4 26.2


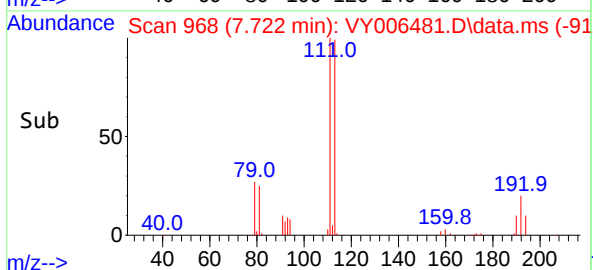
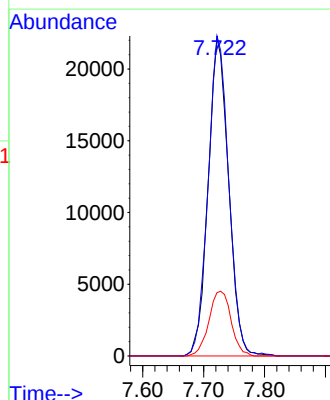
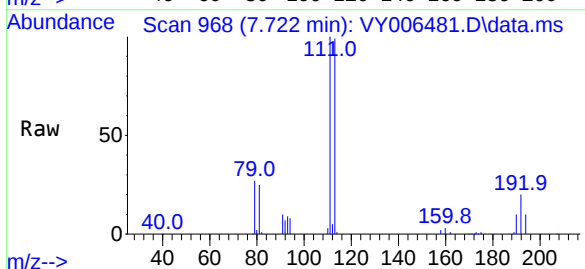


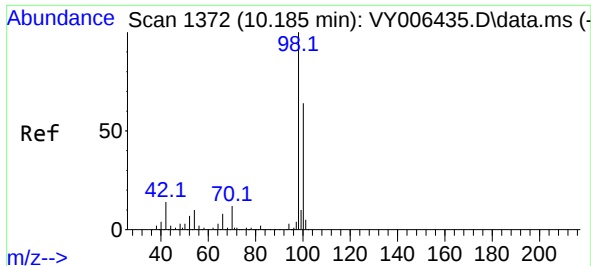

#50
Toluene-d8
Concen: 55.192 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13




Instrument :
MSVOA_Y
ClientSampleId :
PSC124019


Tgt Ion: 98 Resp: 222231
Ion Ratio Lower Upper
98 100
100 62.7 50.9 76.3

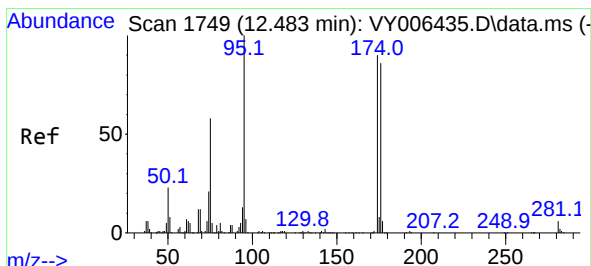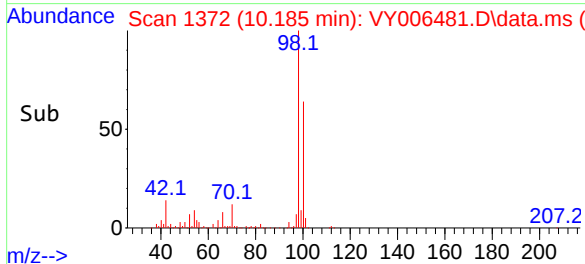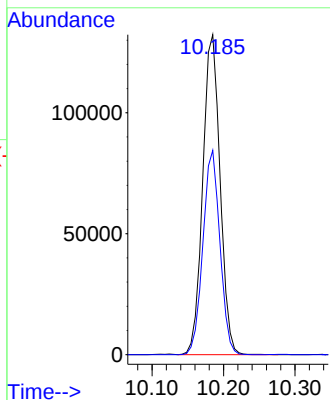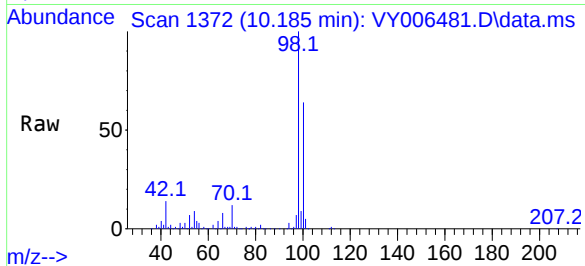

#62
4-Bromofluorobenzene
Concen: 53.354 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13

Tgt Ion: 95 Resp: 72368
Ion Ratio Lower Upper
95 100
174 82.3 0.0 177.0
176 80.0 0.0 169.4


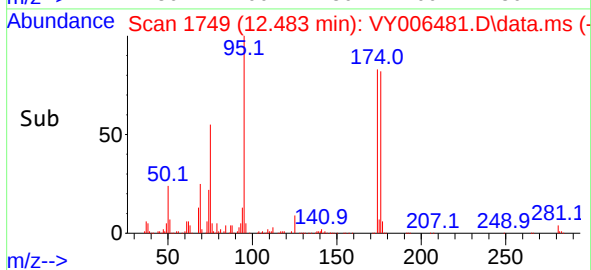
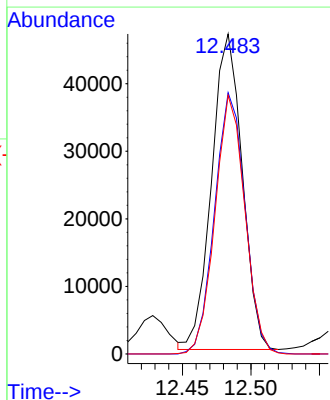
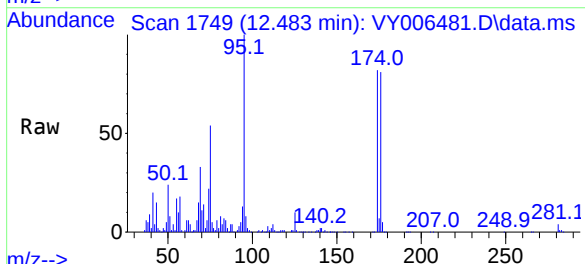


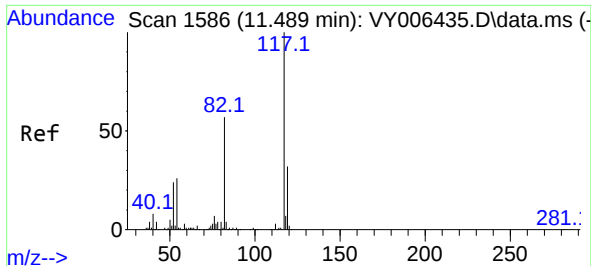

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13

Instrument :
MSVOA_Y
ClientSampleId :
PSC124019

Tgt Ion:117 Resp: 160016
Ion Ratio Lower Upper
117 100
82 57.4 45.7 68.5
119 32.1 25.5 38.3

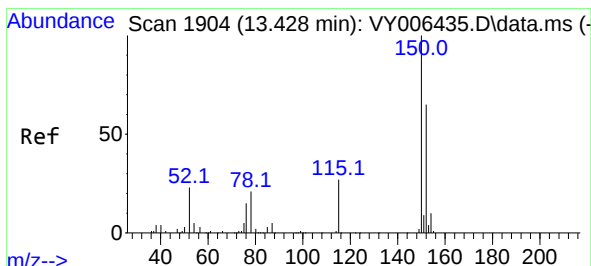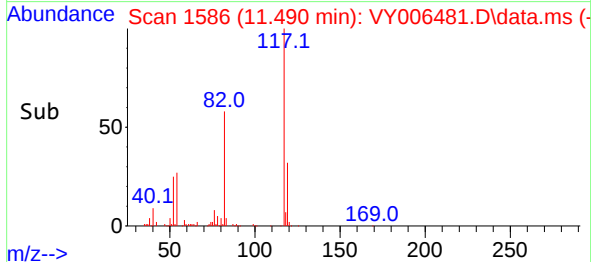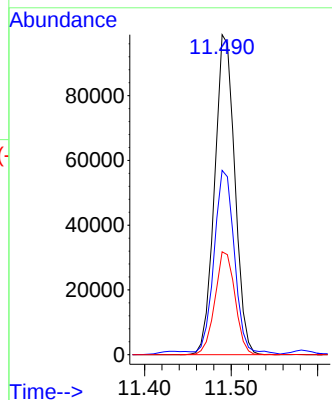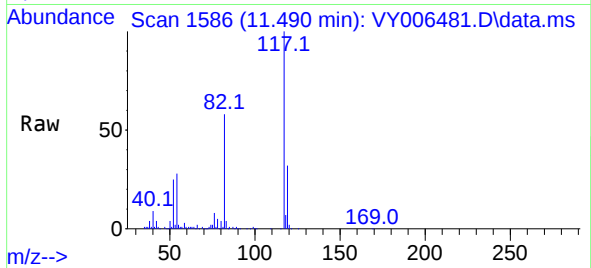

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY006481.D
Acq: 26 Oct 2021 15:13

Tgt Ion:152 Resp: 69911
Ion Ratio Lower Upper
152 100
115 54.0 28.5 85.5
150 150.6 0.0 348.2

