

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102821\
 Data File : VY006520.D
 Acq On : 28 Oct 2021 16:57
 Operator : SY/MD
 Sample : M4373-01
 Misc : 5.05G/5ML/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SU-01-102621

Quant Time: Oct 29 07:05:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 23 06:59:04 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	4508	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	6457	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	7555	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	2780	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	3406	61.398	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 122.800%	
35) Dibromofluoromethane	7.722	113	729	20.256	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 40.520%#	
50) Toluene-d8	10.185	98	8906	58.375	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 116.760%	
62) 4-Bromofluorobenzene	12.483	95	3093	60.183	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 120.360%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.125	50	177	3.147	ug/l #	43
5) Bromomethane	2.674	94	188	4.492	ug/l #	50
10) Methyl Iodide	4.100	142	321	11.557	ug/l #	81
16) Acetone	3.960	43	218	13.648	ug/l #	46
36) 1,1-Dichloropropene	7.789	75	306	4.796	ug/l #	42
38) Carbon Tetrachloride	7.795	117	332	4.717	ug/l #	12
48) Methyl methacrylate	9.288	41	67	1.846	ug/l #	16
51) 4-Methyl-2-Pentanone	10.069	43	305	7.428	ug/l #	39
55) 1,1,2-Trichloroethane	10.654	97	83	2.426	ug/l #	39
56) Ethyl methacrylate	10.532	69	153	2.895	ug/l #	50
59) 2-Hexanone	10.837	43	122	4.105	ug/l #	28
60) Dibromochloromethane	10.953	129	44	1.043	ug/l #	10
66) 1,1,1,2-Tetrachloroethane	11.581	131	59	1.066	ug/l #	1
67) Ethyl Benzene	11.617	91	351	1.254	ug/l #	44
71) Bromoform	12.178	173	109	3.115	ug/l #	88
73) Isopropylbenzene	12.324	105	243	1.250	ug/l	76
74) N-amyl acetate	12.123	43	152	2.356	ug/l #	13
75) 1,1,2,2-Tetrachloroethane	12.550	83	119	3.535	ug/l #	1
76) 1,2,3-Trichloropropane	12.483	75	1835	64.055	ug/l #	100
77) Bromobenzene	12.446	156	180	3.929	ug/l #	1
78) n-propylbenzene	12.757	91	292	1.215	ug/l	98
79) 2-Chlorotoluene	12.757	91	294	2.210	ug/l #	41
81) trans-1,4-Dichloro-2-b...	12.483	75	1835	131.503	ug/l #	12
82) 4-Chlorotoluene	12.861	91	464	3.347	ug/l #	41
83) tert-Butylbenzene	13.056	119	442	3.159	ug/l #	25
84) 1,2,4-Trimethylbenzene	13.111	105	2143	13.162	ug/l #	31
88) 1,4-Dichlorobenzene	13.446	146	118	1.305	ug/l #	1
89) n-Butylbenzene	13.690	91	211	1.251	ug/l #	61
90) Hexachloroethane	13.977	117	113	3.491	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.379	75	20	2.798	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102821\
Data File : VY006520.D
Acq On : 28 Oct 2021 16:57
Operator : SY/MD
Sample : M4373-01
Misc : 5.05G/5ML/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Quant Time: Oct 29 07:05:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
Quant Title : SW846 8260
QLast Update : Sat Oct 23 06:59:04 2021
Response via : Initial Calibration

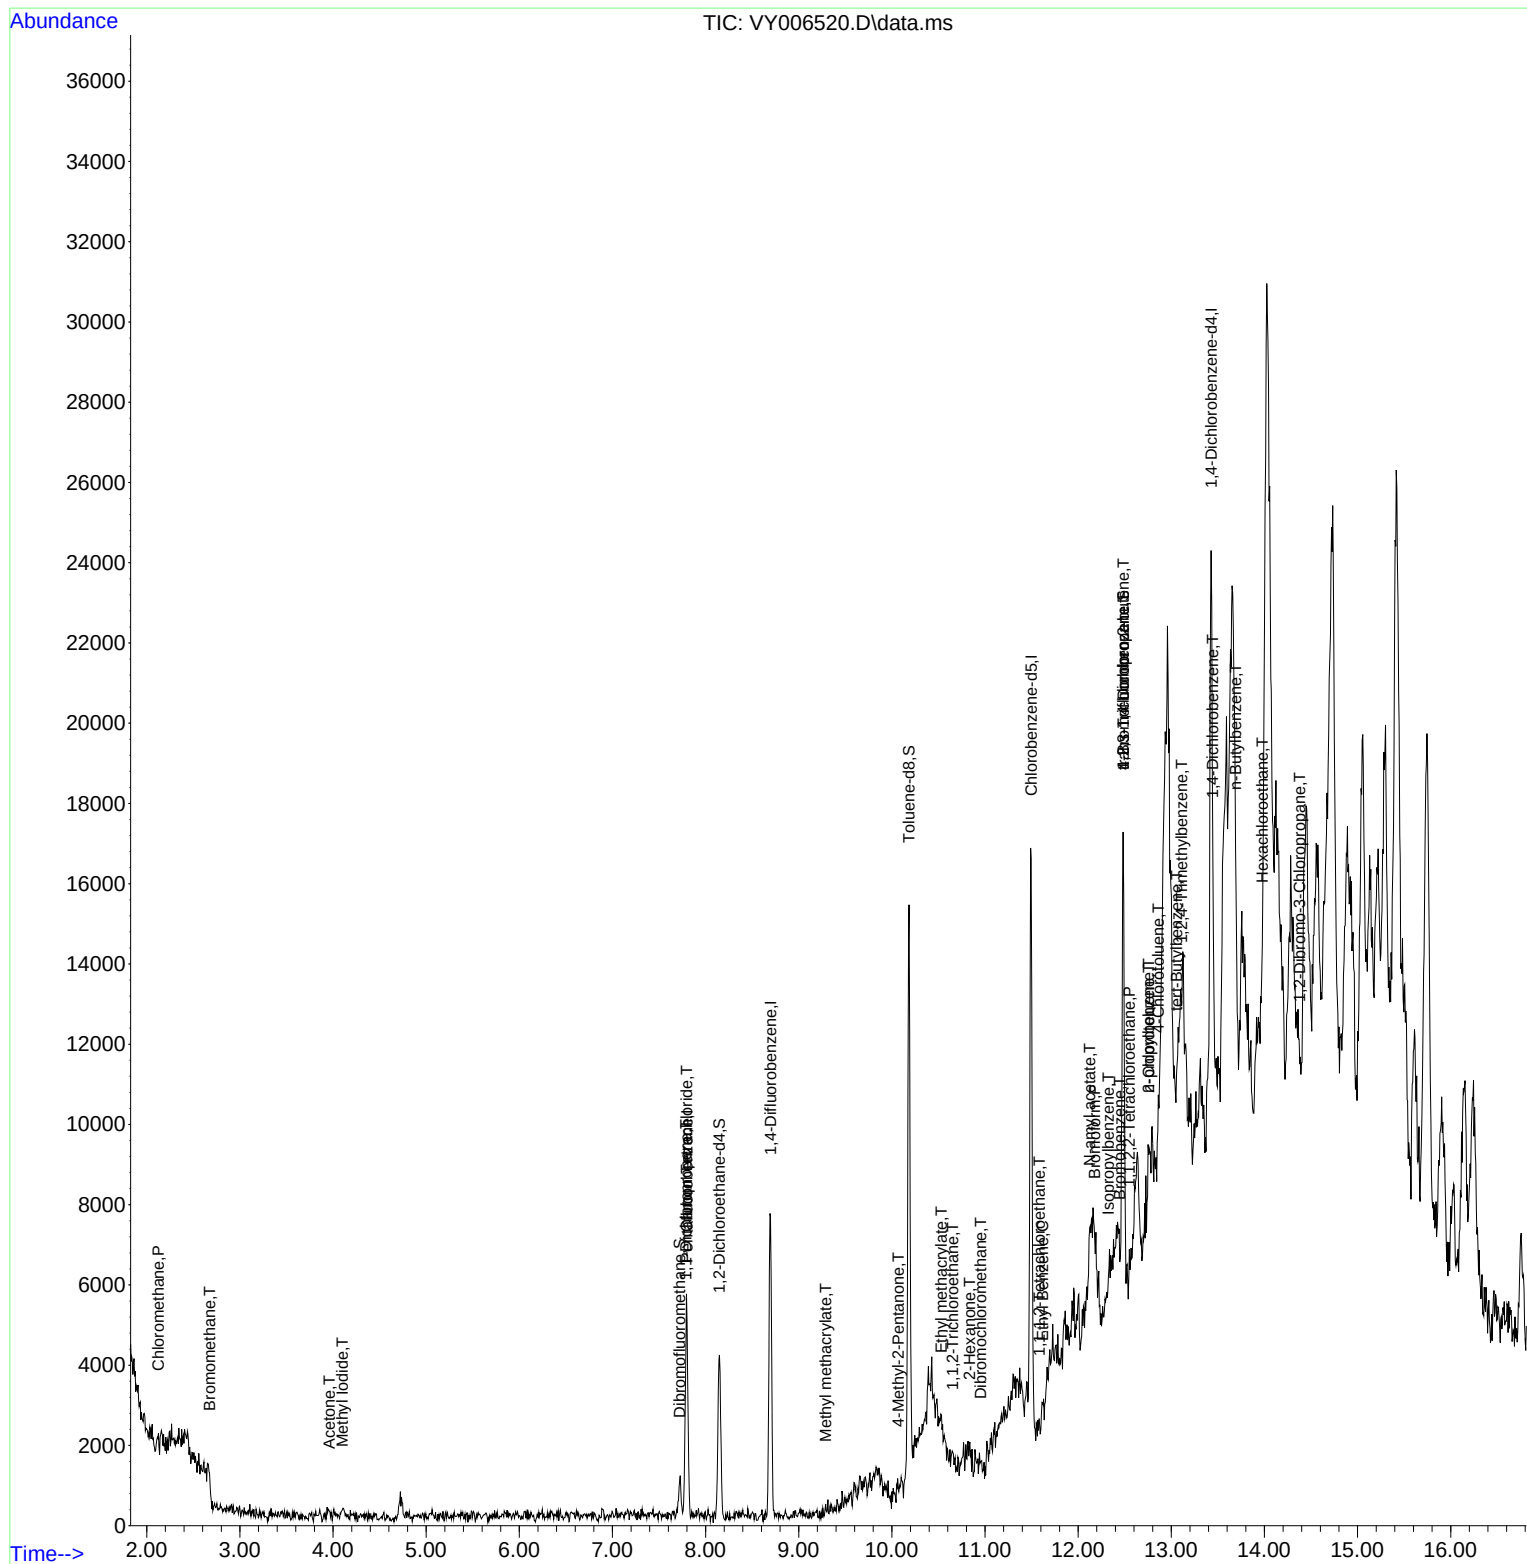






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621







Tgt Ion:168 Resp: 4508
Ion Ratio Lower Upper
168 100
99 44.9 44.8 67.2

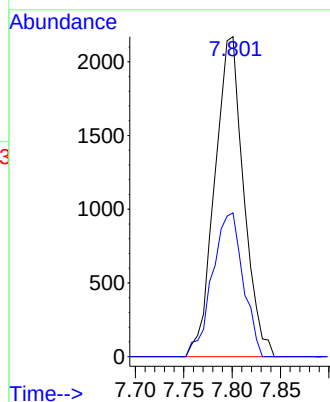

#3
Chloromethane
Concen: 3.147 ug/l
RT: 2.125 min Scan# 50
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 50 Resp: 177
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#


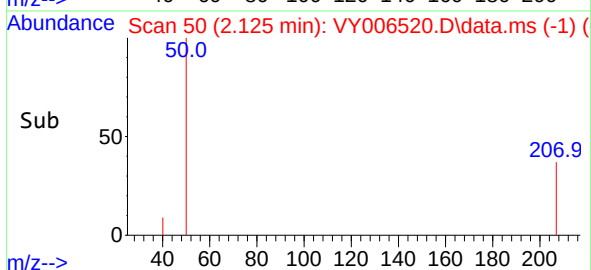




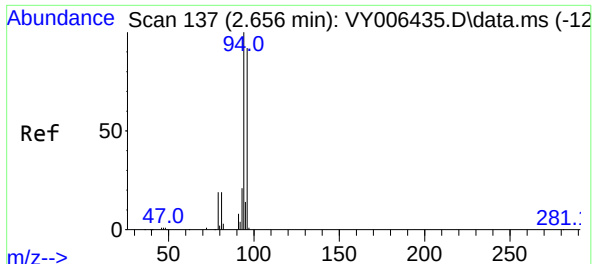

#5
Bromomethane
Concen: 4.492 ug/l
RT: 2.674 min Scan# 140
Delta R.T. 0.018 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 94 Resp: 188
Ion Ratio Lower Upper
94 100
96 44.7 73.5 110.3#

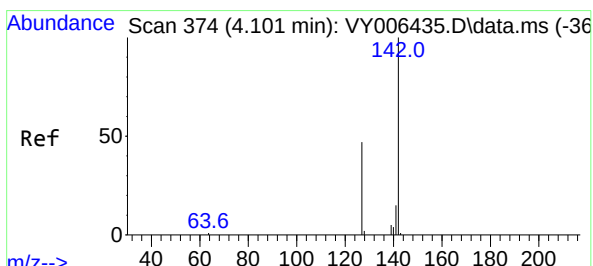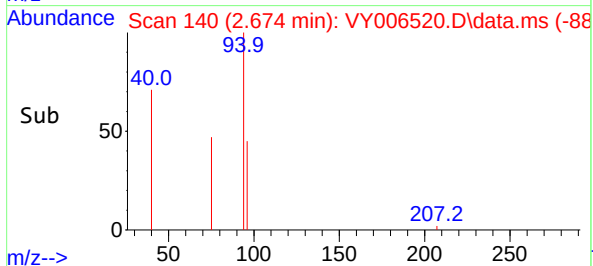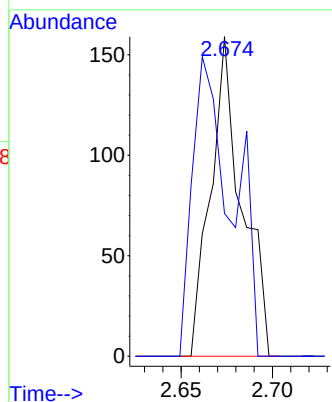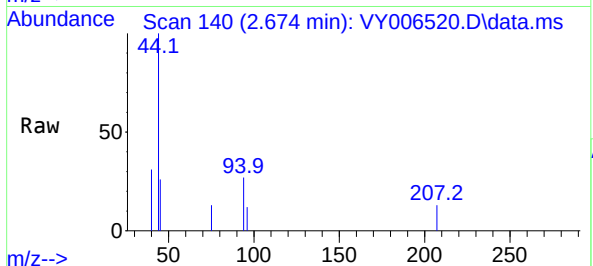

#10
Methyl Iodide
Concen: 11.557 ug/l
RT: 4.100 min Scan# 374
Delta R.T. -0.001 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 142 Resp: 321
Ion Ratio Lower Upper
142 100
127 40.8 40.1 60.1
141 0.0 12.5 18.7#


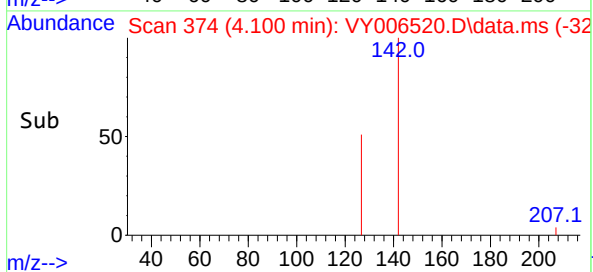
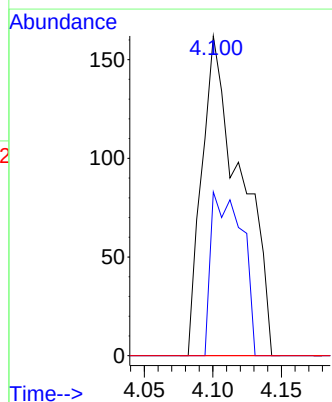
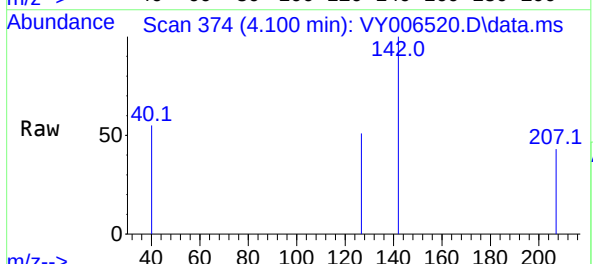


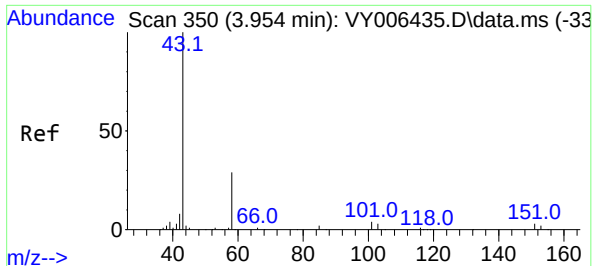

#16
Acetone
Concen: 13.648 ug/l
RT: 3.960 min Scan# 351
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 43 Resp: 218
Ion Ratio Lower Upper
43 100
58 0.0 22.9 34.3#

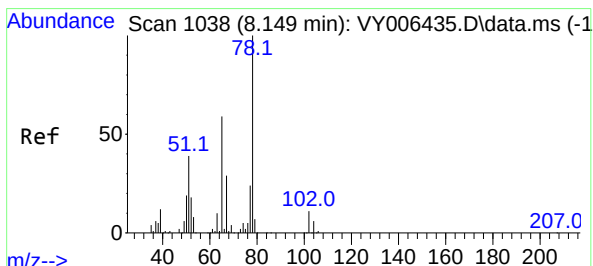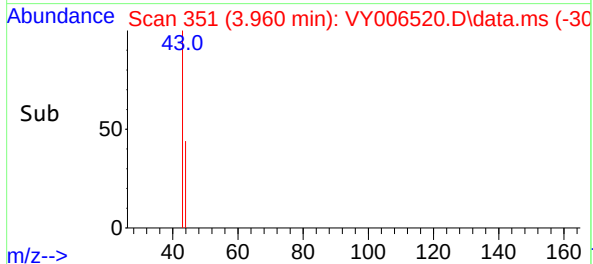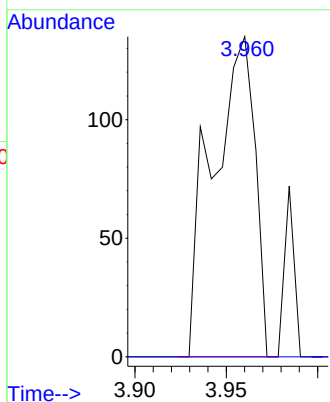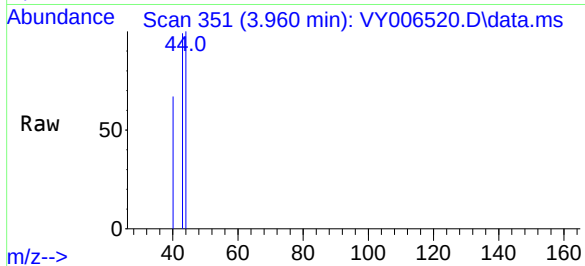

#33
1,2-Dichloroethane-d4
Concen: 61.398 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 65 Resp: 3406
Ion Ratio Lower Upper
65 100
67 47.7 0.0 98.2


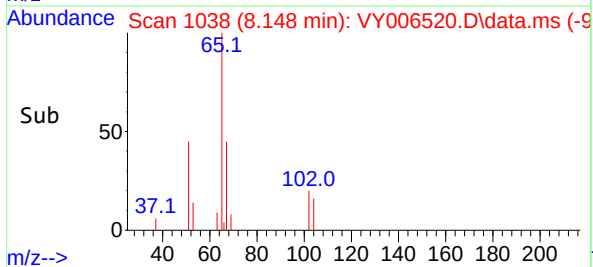

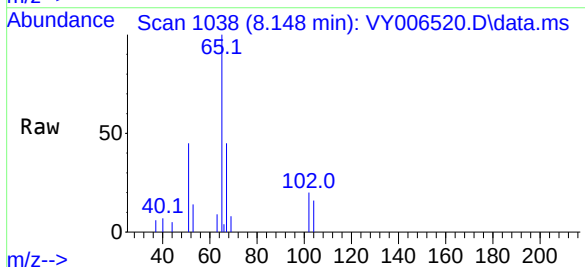




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion:	114	Resp:	6457
Ion	Ratio	Lower	Upper
114	100		
63	24.6	0.0	45.0
88	14.6	0.0	30.6

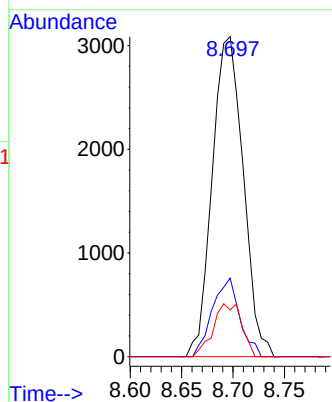

#35
Dibromofluoromethane
Concen: 20.256 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion:	113	Resp:	729
Ion	Ratio	Lower	Upper
113	100		
111	97.4	82.3	123.5
192	12.5	17.4	26.2#


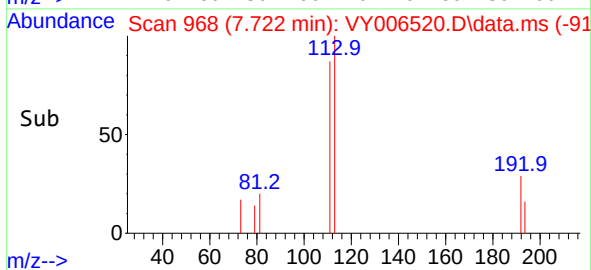




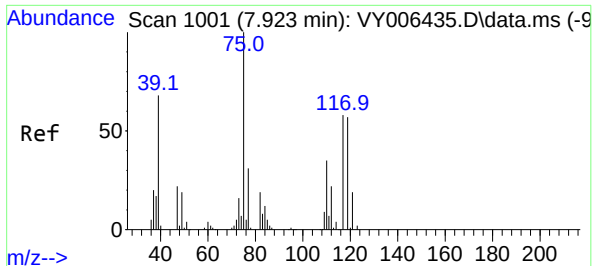

#36
1,1-Dichloropropene
Concen: 4.796 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.134 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 75 Resp: 306
Ion Ratio Lower Upper
75 100
110 0.0 17.1 51.3#
77 0.0 24.9 37.3#

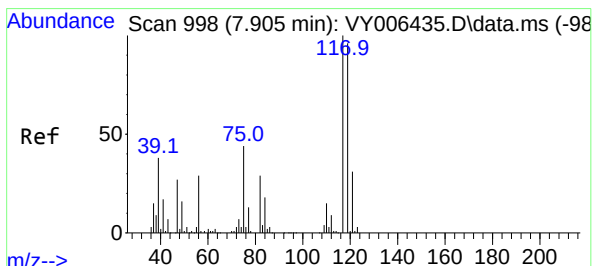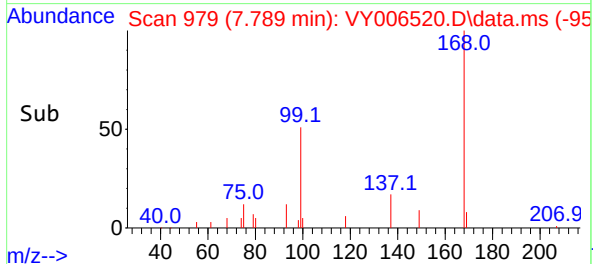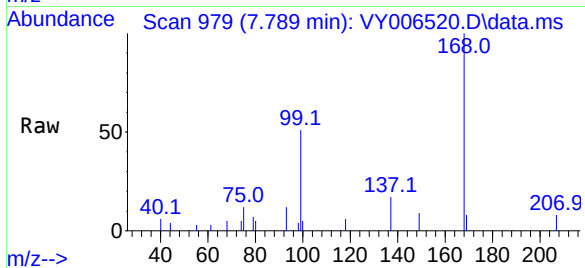

#38
Carbon Tetrachloride
Concen: 4.717 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.110 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 117 Resp: 332
Ion Ratio Lower Upper
117 100
119 0.0 76.6 115.0#
121 0.0 24.7 37.1#


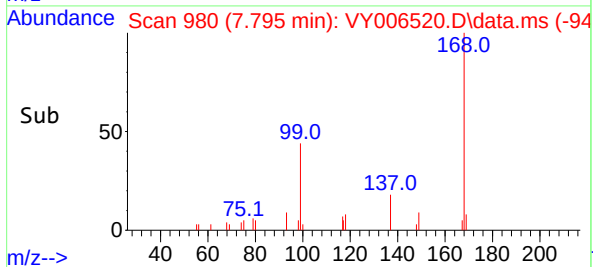

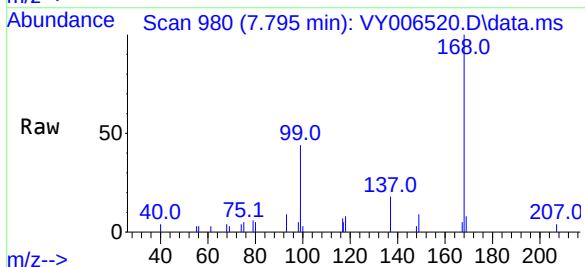


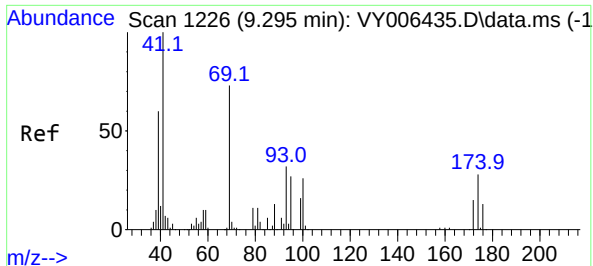

#48
Methyl methacrylate
Concen: 1.846 ug/l
RT: 9.288 min Scan# 1225
Delta R.T. -0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 41 Resp: 67
Ion Ratio Lower Upper
41 100
69 0.0 60.4 90.6#
39 0.0 48.2 72.2#

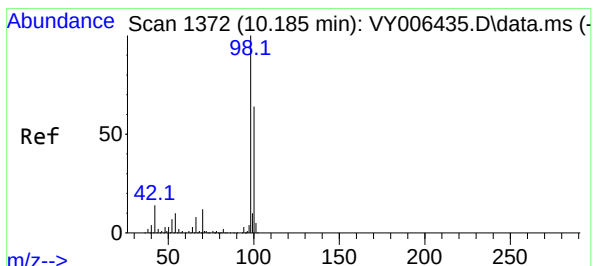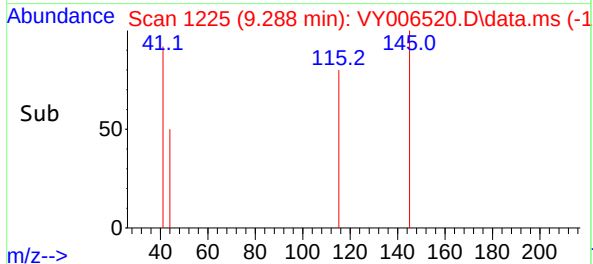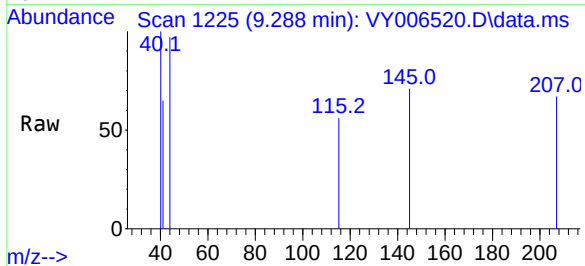

#50
Toluene-d8
Concen: 58.375 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 98 Resp: 8906
Ion Ratio Lower Upper
98 100
100 62.2 50.9 76.3


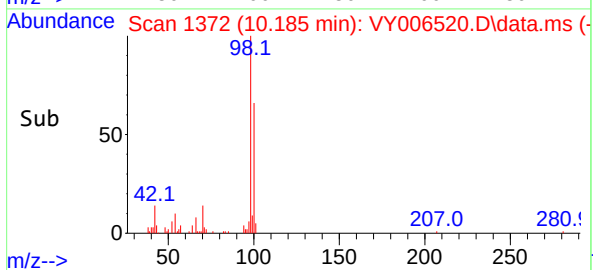

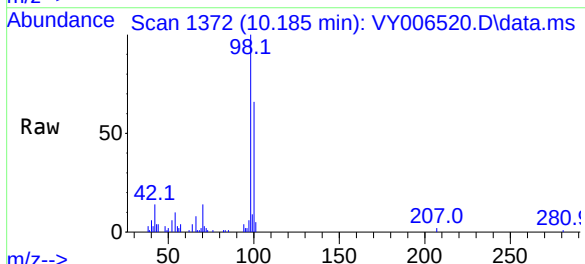




#51
4-Methyl-2-Pentanone
Concen: 7.428 ug/l
RT: 10.069 min Scan# 1353
Delta R.T. -0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 43 Resp: 305
Ion Ratio Lower Upper
43 100
58 0.0 28.7 43.1#

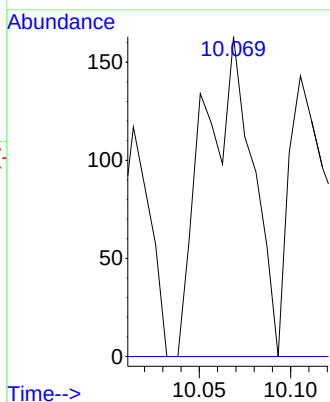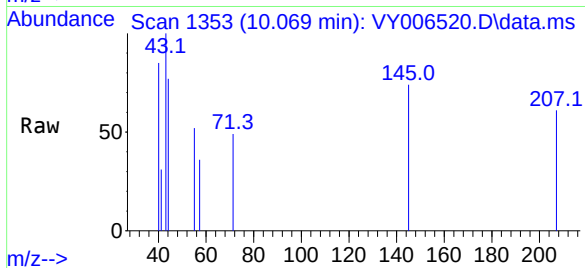

#55
1,1,2-Trichloroethane
Concen: 2.426 ug/l
RT: 10.654 min Scan# 1449
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 97 Resp: 83
Ion Ratio Lower Upper
97 100
83 53.7 66.2 99.2#
85 113.7 42.2 63.4#
99 0.0 48.6 73.0#


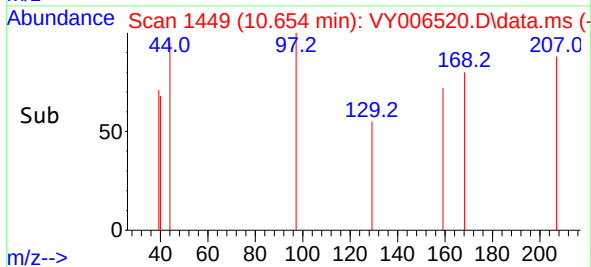

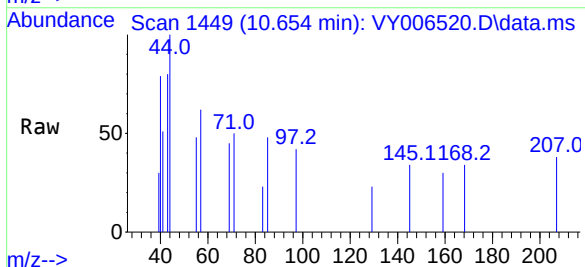




#56
Ethyl methacrylate
Concen: 2.895 ug/l
RT: 10.532 min Scan# 1429
Delta R.T. 0.018 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 69 Resp: 153
Ion Ratio Lower Upper
69 100
41 43.8 62.9 94.3#
39 0.0 35.7 53.5#

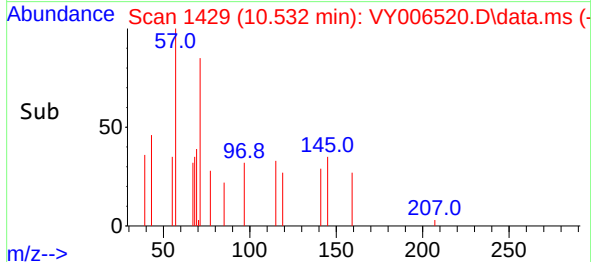

#59
2-Hexanone
Concen: 4.105 ug/l
RT: 10.837 min Scan# 1479
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 43 Resp: 122
Ion Ratio Lower Upper
43 100
58 0.0 24.6 73.6#


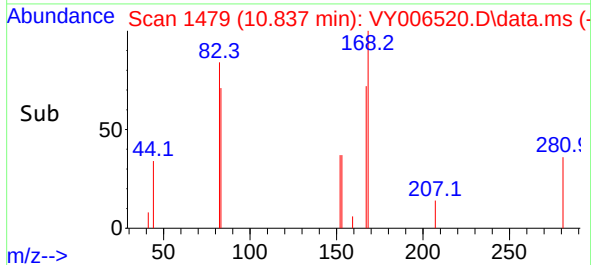

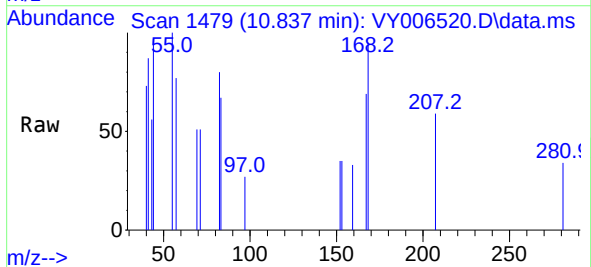




#60
Dibromochloromethane
Concen: 1.043 ug/l
RT: 10.953 min Scan# 1498
Delta R.T. -0.031 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion:129 Resp: 44
Ion Ratio Lower Upper
129 100
127 0.0 39.4 118.1#

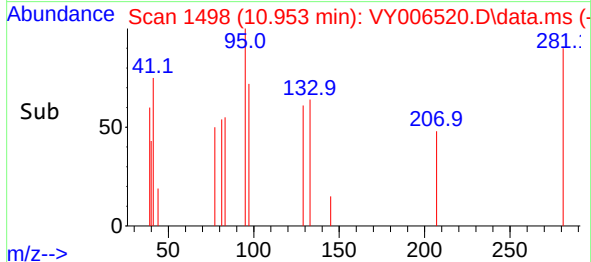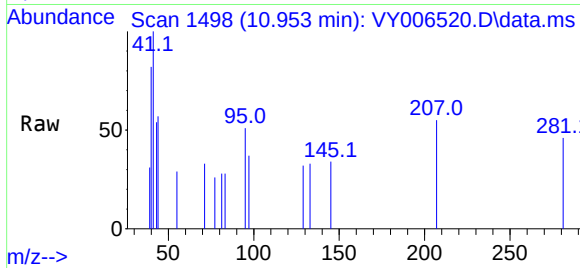

#62
4-Bromofluorobenzene
Concen: 60.183 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 95 Resp: 3093
Ion Ratio Lower Upper
95 100
174 90.4 0.0 177.0
176 84.5 0.0 169.4


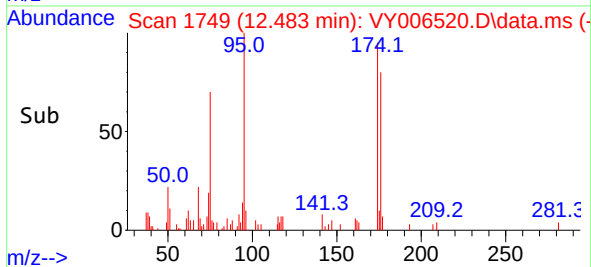

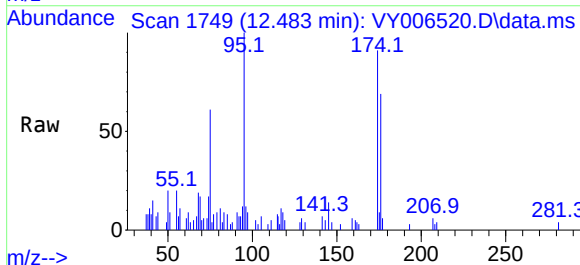




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampled :
SU-01-102621


Tgt Ion:117	Resp:	7555
Ion	Ratio	Lower Upper
117	100	
82	52.4	45.7 68.5
119	34.0	25.5 38.3

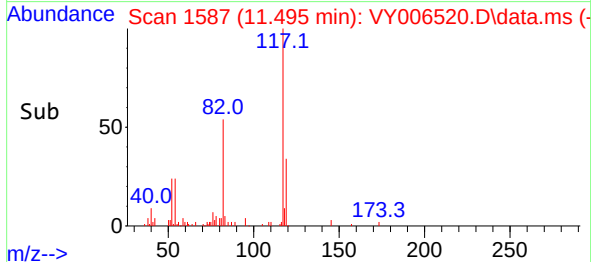

#66
1,1,1,2-Tetrachloroethane
Concen: 1.066 ug/l
RT: 11.581 min Scan# 1601
Delta R.T. -0.012 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion:131	Resp:	59
Ion	Ratio	Lower Upper
131	100	
133	0.0	47.8 143.3#
119	215.3	30.8 92.4#


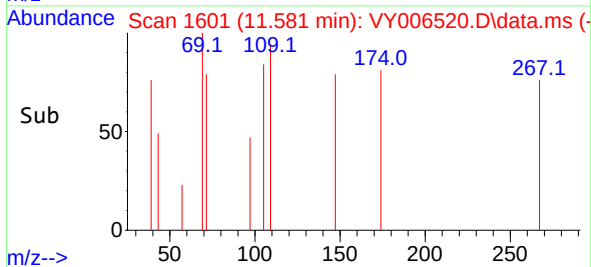

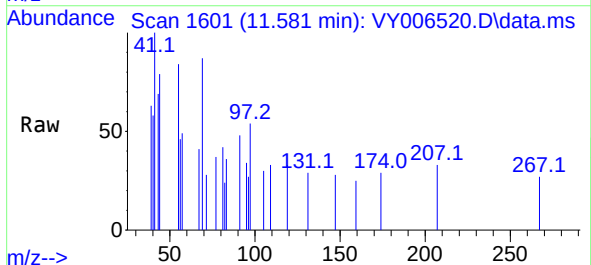




#67
Ethyl Benzene
Concen: 1.254 ug/l
RT: 11.617 min Scan# 1607
Delta R.T. 0.024 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampled :
SU-01-102621


Tgt Ion: 91 Resp: 351
Ion Ratio Lower Upper
91 100
106 0.0 24.2 36.4#



#71
Bromoform
Concen: 3.115 ug/l
RT: 12.178 min Scan# 1699
Delta R.T. -0.031 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 173 Resp: 109
Ion Ratio Lower Upper
173 100
175 41.3 24.8 74.3
254 0.0 0.1 0.1#


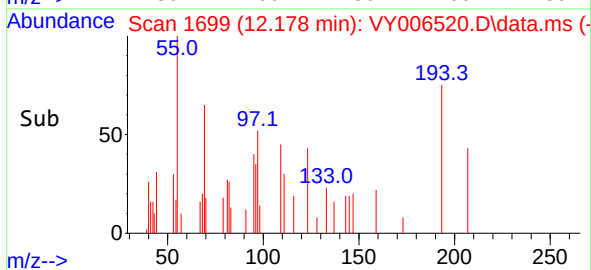






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion:	152	Resp:	2780
Ion	Ratio	Lower	Upper
152	100		
115	60.8	28.5	85.5
150	142.9	0.0	348.2

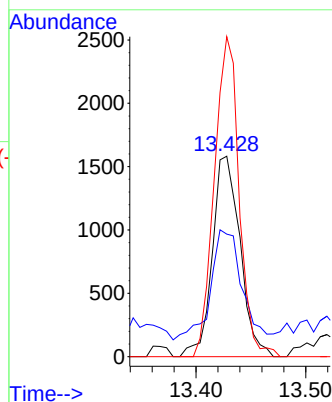

#73
Isopropylbenzene
Concen: 1.250 ug/l
RT: 12.324 min Scan# 1723
Delta R.T. -0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57


Tgt Ion:	105	Resp:	243
Ion	Ratio	Lower	Upper
105	100		
120	39.1	13.3	39.9

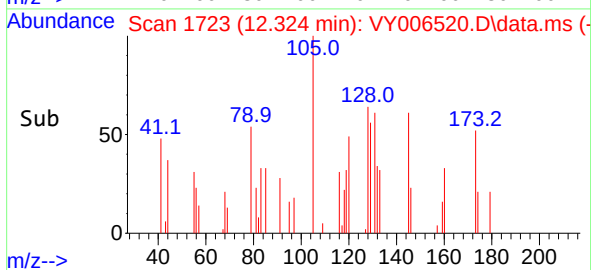






#74
N-amy1 acetate
Concen: 2.356 ug/l
RT: 12.123 min Scan# 1690
Delta R.T. -0.019 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621

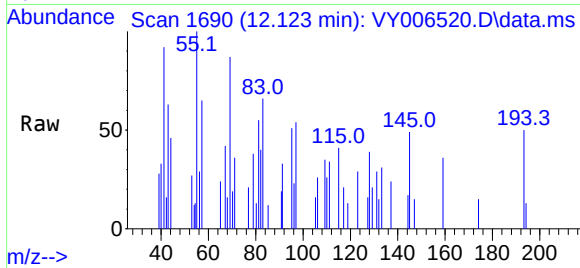

Tgt Ion: 43 Resp: 152




Ion	Ratio	Lower	Upper
43	100		
70	117.1	29.4	44.0#
55	0.0	18.1	27.1#
61	0.0	17.6	26.4#

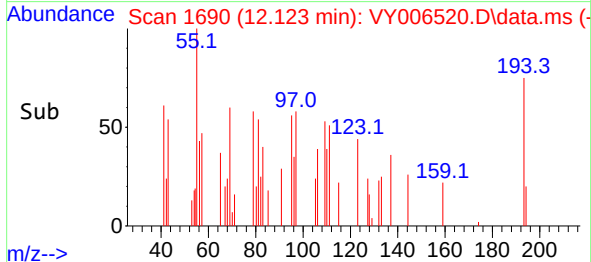


#75
1,1,2,2-Tetrachloroethane
Concen: 3.535 ug/l
RT: 12.550 min Scan# 1760
Delta R.T. -0.031 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 83 Resp: 119

Ion	Ratio	Lower	Upper
83	100		
131	149.6	5.5	16.4#
85	147.1	31.9	95.9#


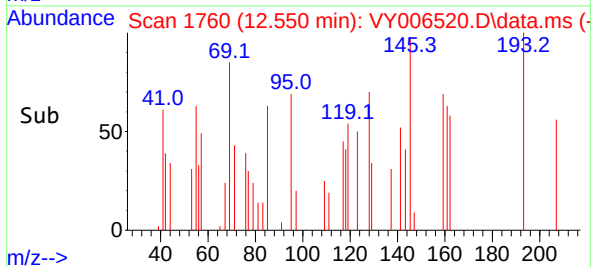
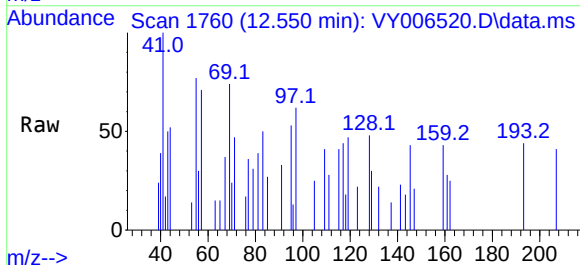





#76
1,2,3-Trichloropropane
Concen: 64.055 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.153 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 75 Resp: 1835
Ion Ratio Lower Upper
75 100
77 2.1 0.0 0.0#

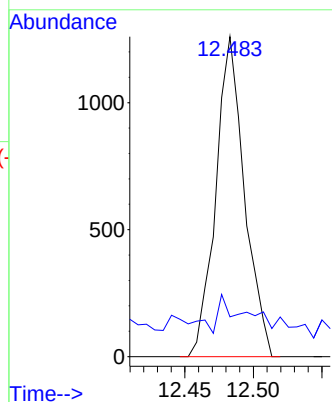

#77
Bromobenzene
Concen: 3.929 ug/l
RT: 12.446 min Scan# 1743
Delta R.T. -0.165 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion:156 Resp: 180
Ion Ratio Lower Upper
156 100
77 33.9 94.2 282.4#
158 0.0 48.6 145.8#


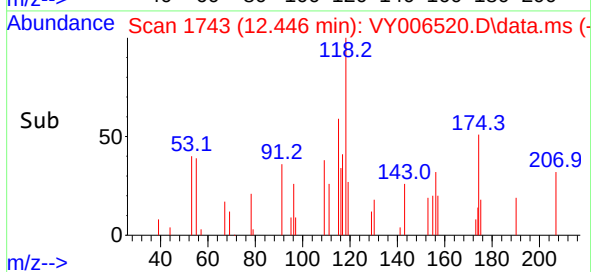
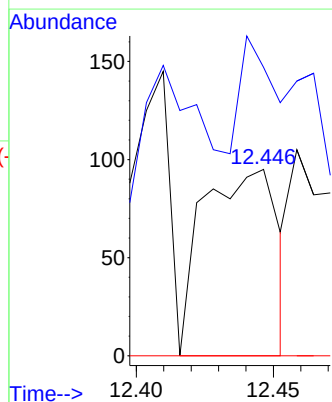





#78
n-propylbenzene
Concen: 1.215 ug/l
RT: 12.757 min Scan# 1794
Delta R.T. 0.085 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampled :
SU-01-102621


Tgt Ion: 91 Resp: 292
Ion Ratio Lower Upper
91 100
120 21.6 11.3 33.8

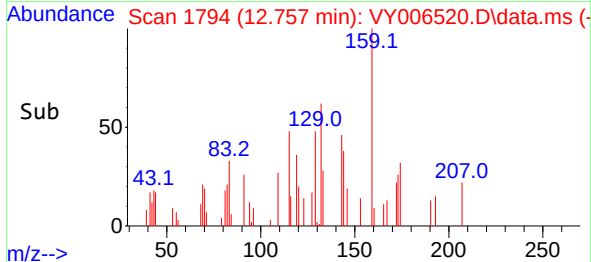

#79
2-Chlorotoluene
Concen: 2.210 ug/l
RT: 12.757 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 91 Resp: 294
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#


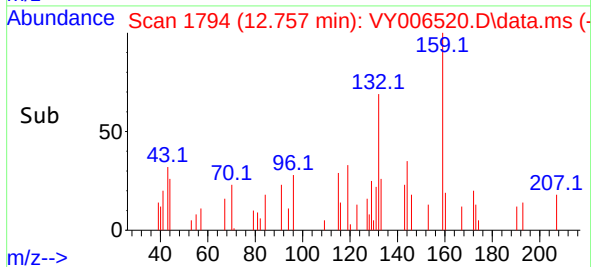

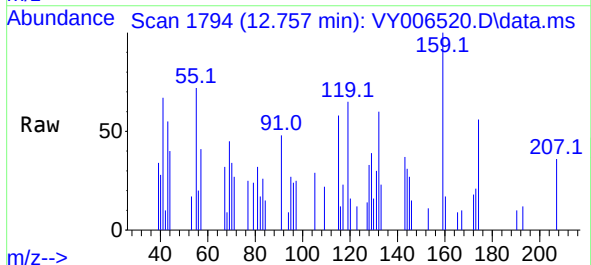




#81
trans-1,4-Dichloro-2-butene
Concen: 131.503 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.103 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion: 75 Resp: 1835
Ion Ratio Lower Upper
75 100
53 7.4 85.8 128.6#
89 0.0 39.3 58.9#

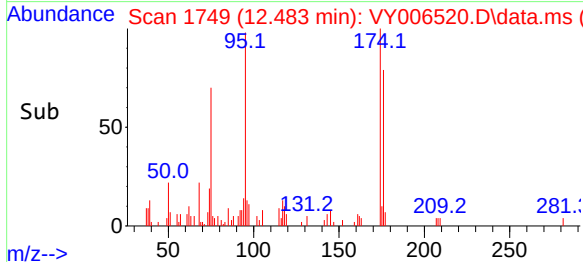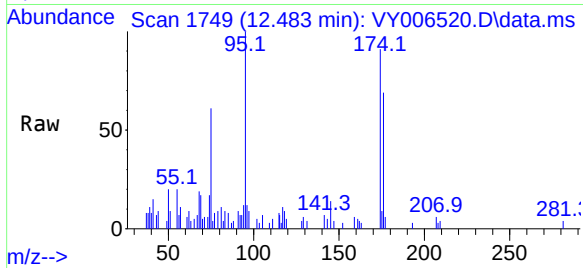

#82
4-Chlorotoluene
Concen: 3.347 ug/l
RT: 12.861 min Scan# 1811
Delta R.T. 0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 91 Resp: 464
Ion Ratio Lower Upper
91 100
126 0.0 16.8 50.4#


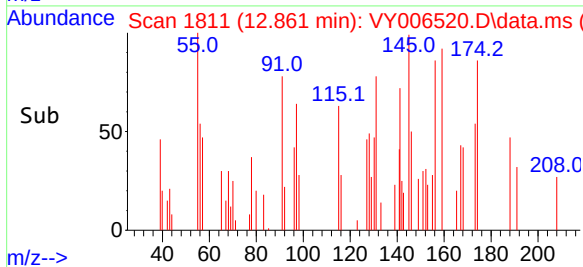

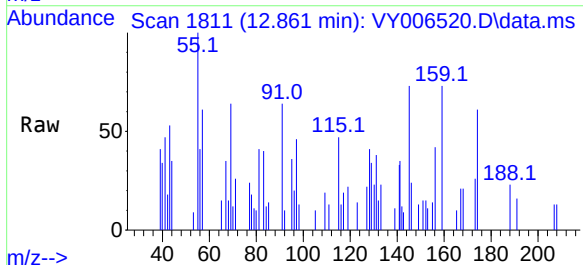




#83
tert-Butylbenzene
Concen: 3.159 ug/l
RT: 13.056 min Scan# 1843
Delta R.T. -0.019 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57




Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621


Tgt Ion:119 Resp: 442
Ion Ratio Lower Upper
119 100
91 0.0 34.8 104.5#
134 50.2 13.0 38.9#



#84
1,2,4-Trimethylbenzene
Concen: 13.162 ug/l
RT: 13.111 min Scan# 1852
Delta R.T. -0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57


Tgt Ion:105 Resp: 2143
Ion Ratio Lower Upper
105 100
120 0.0 22.6 67.8#

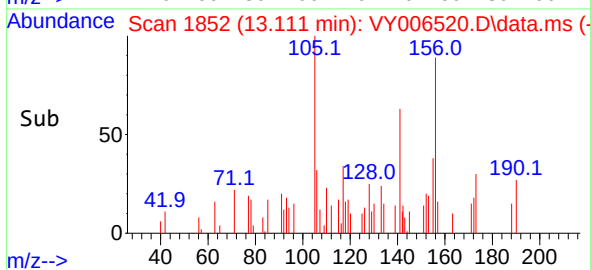






#88
1,4-Dichlorobenzene
Concen: 1.305 ug/l
RT: 13.446 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Instrument :
MSVOA_Y
ClientSampled :
SU-01-102621







Tgt Ion:146 Resp: 118
Ion Ratio Lower Upper
146 100
111 317.8 18.9 56.5#
148 0.0 32.0 96.2#

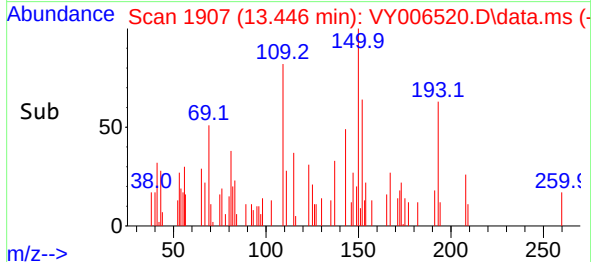

#89
n-Butylbenzene
Concen: 1.251 ug/l
RT: 13.690 min Scan# 1947
Delta R.T. -0.006 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 91 Resp: 211
Ion Ratio Lower Upper
91 100
92 76.3 26.3 78.9
134 0.0 12.9 38.7#


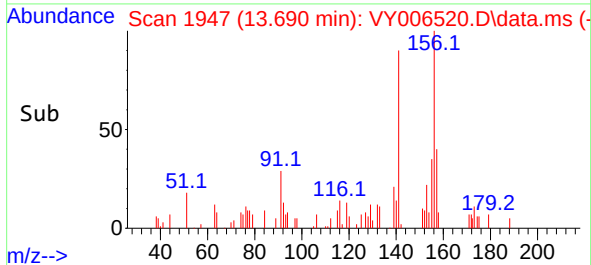

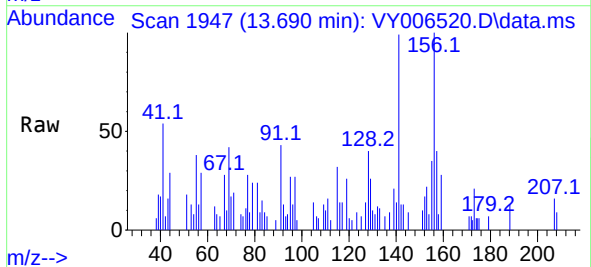




#90
Hexachloroethane
Concen: 3.491 ug/l
RT: 13.977 min Scan# 1994
Delta R.T. 0.018 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Instrument :
MSVOA_Y
ClientSampleId :
SU-01-102621

Tgt Ion:117 Resp: 113
Ion Ratio Lower Upper
117 100
201 0.0 43.4 130.1#

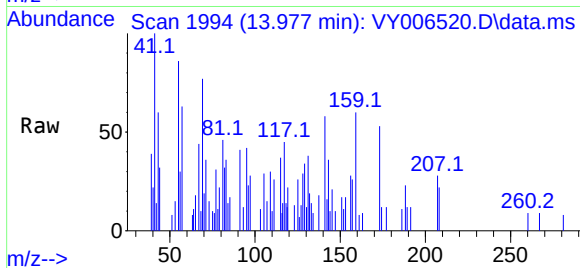

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.798 ug/l
RT: 14.379 min Scan# 2060
Delta R.T. 0.024 min
Lab File: VY006520.D
Acq: 28 Oct 2021 16:57

Tgt Ion: 75 Resp: 20
Ion Ratio Lower Upper
75 100
155 205.0 39.0 116.9#
157 0.0 49.2 147.6#

