
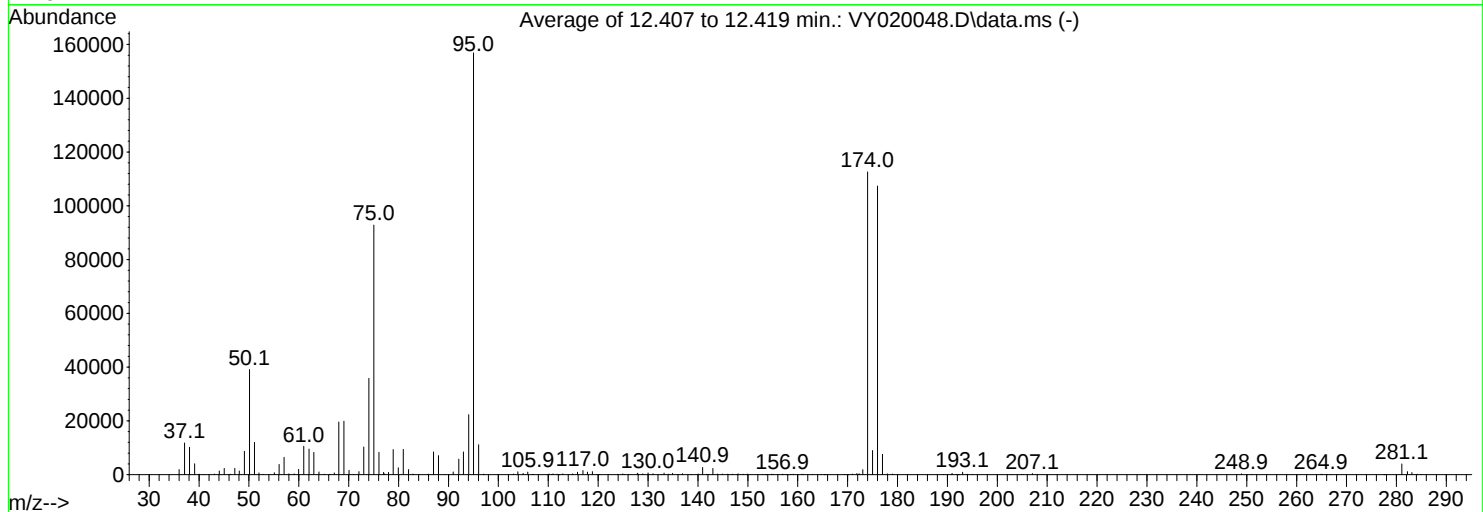


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102924\
Data File : VY020048.D
Acq On : 29 Oct 2024 08:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Wed Oct 16 05:44:48 2024

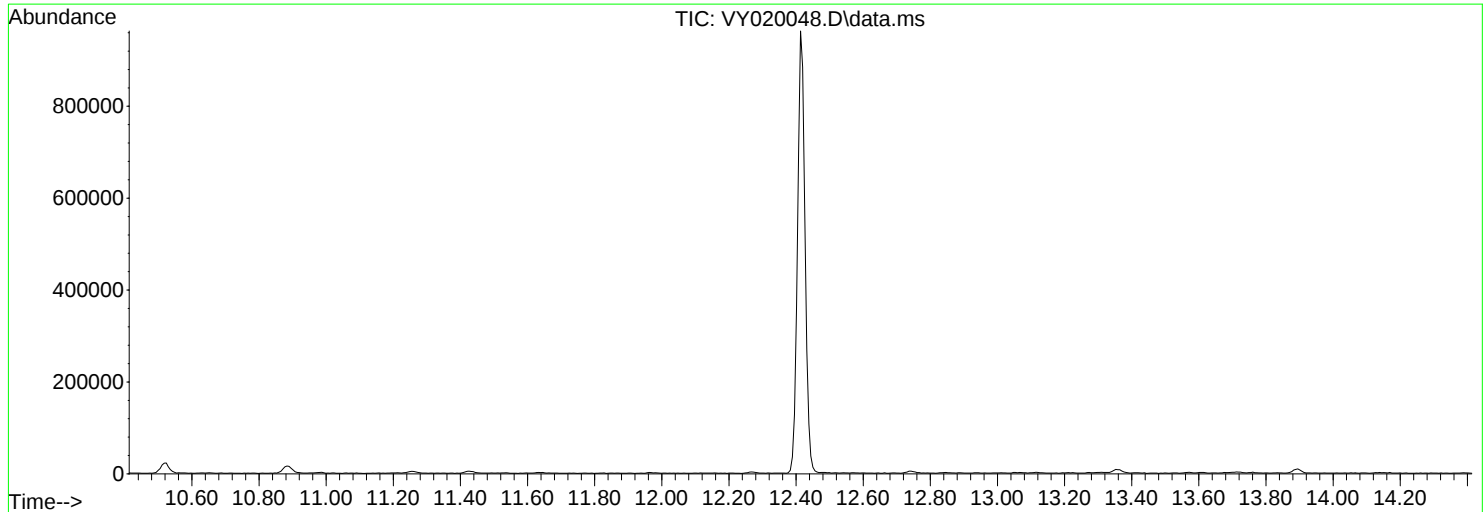

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	39088	PASS
75	95	30	60	59.2	92827	PASS
95	95	100	100	100.0	156885	PASS
96	95	5	9	7.1	11123	PASS
173	174	0.00	2	1.6	1851	PASS
174	95	50	100	71.8	112619	PASS
175	174	5	9	8.0	9023	PASS
176	174	95	101	95.3	107336	PASS
177	176	5	9	7.1	7591	PASS