
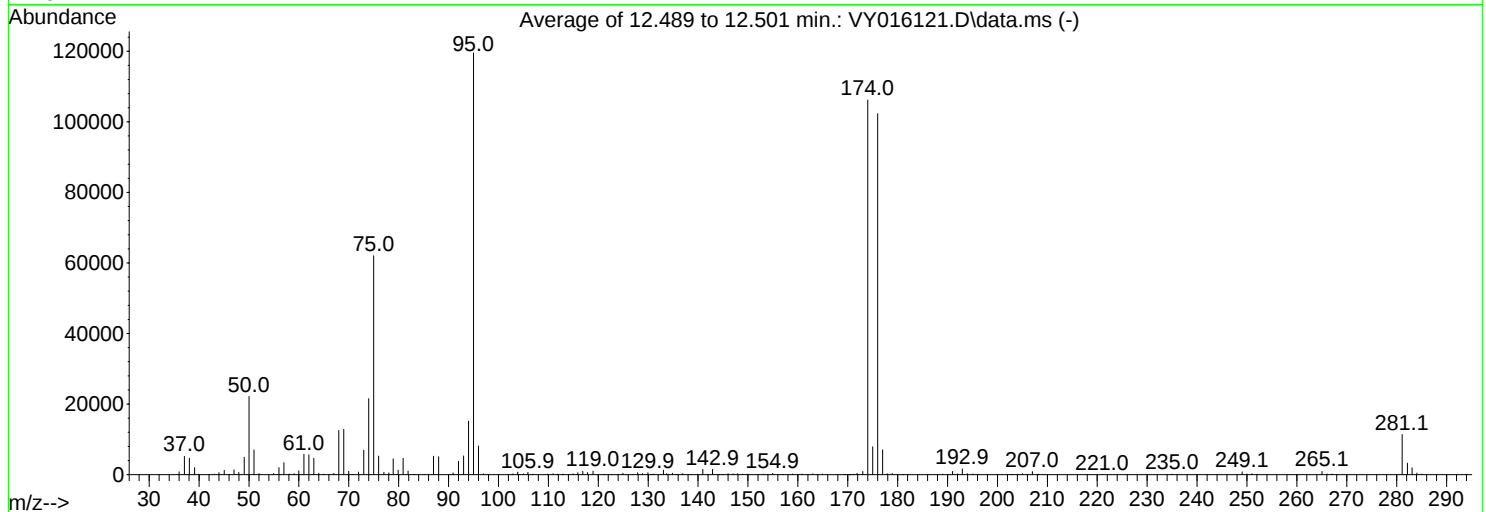


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY103023\
Data File : VY016121.D
Acq On : 30 Oct 2023 08:37
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102623S.M
Title : SW846 8260
Last Update : Fri Oct 27 04:12:29 2023

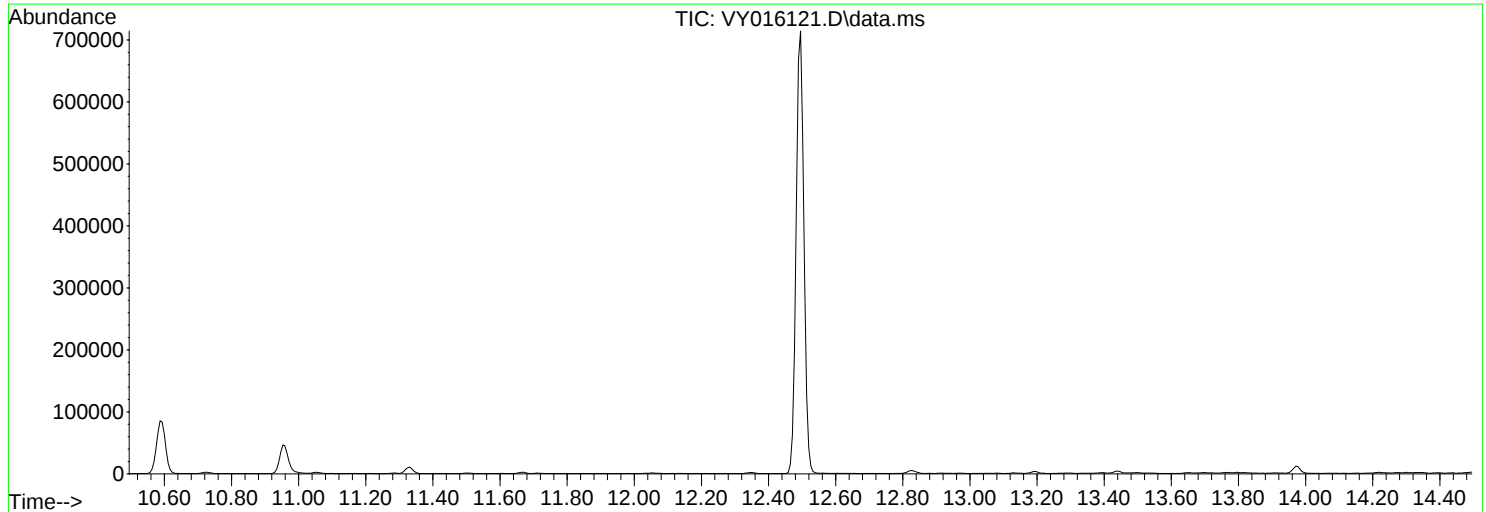

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	22176	PASS
75	95	30	60	51.9	62048	PASS
95	95	100	100	100.0	119552	PASS
96	95	5	9	6.8	8142	PASS
173	174	0.00	2	0.8	896	PASS
174	95	50	100	88.8	106187	PASS
175	174	5	9	7.4	7877	PASS
176	174	95	101	96.4	102315	PASS
177	176	5	9	6.9	7054	PASS