
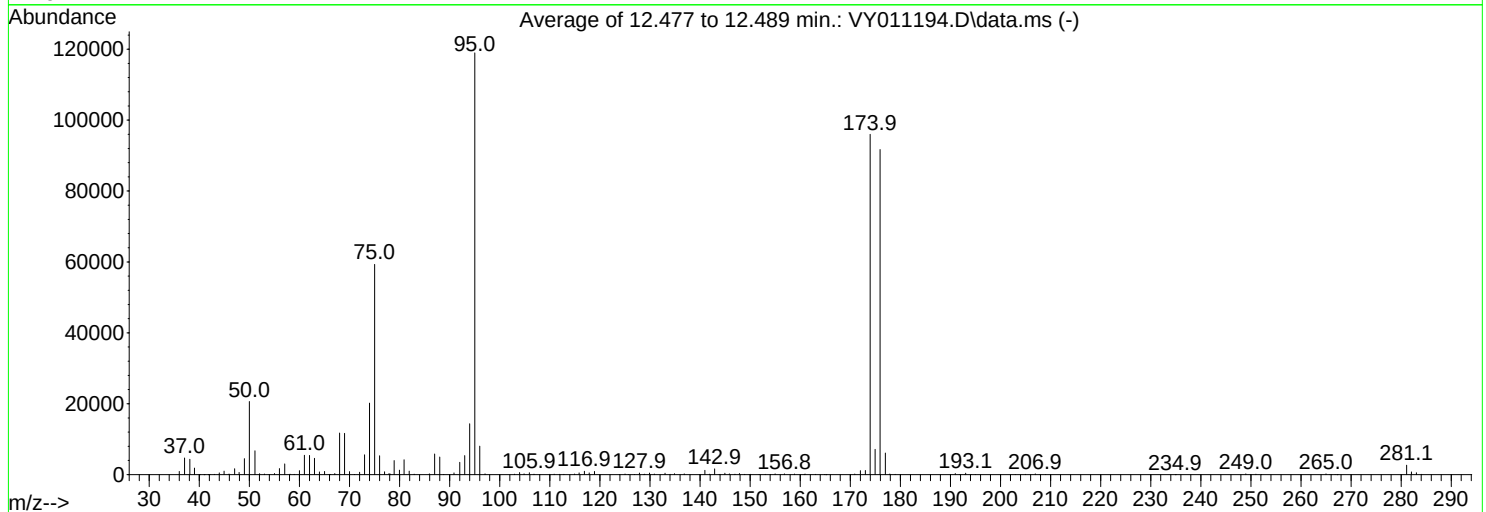


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY103122\
 Data File : VY011194.D
 Acq On : 31 Oct 2022 11:06
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102822S.M
 Title : SW846 8260
 Last Update : Fri Oct 28 23:42:14 2022

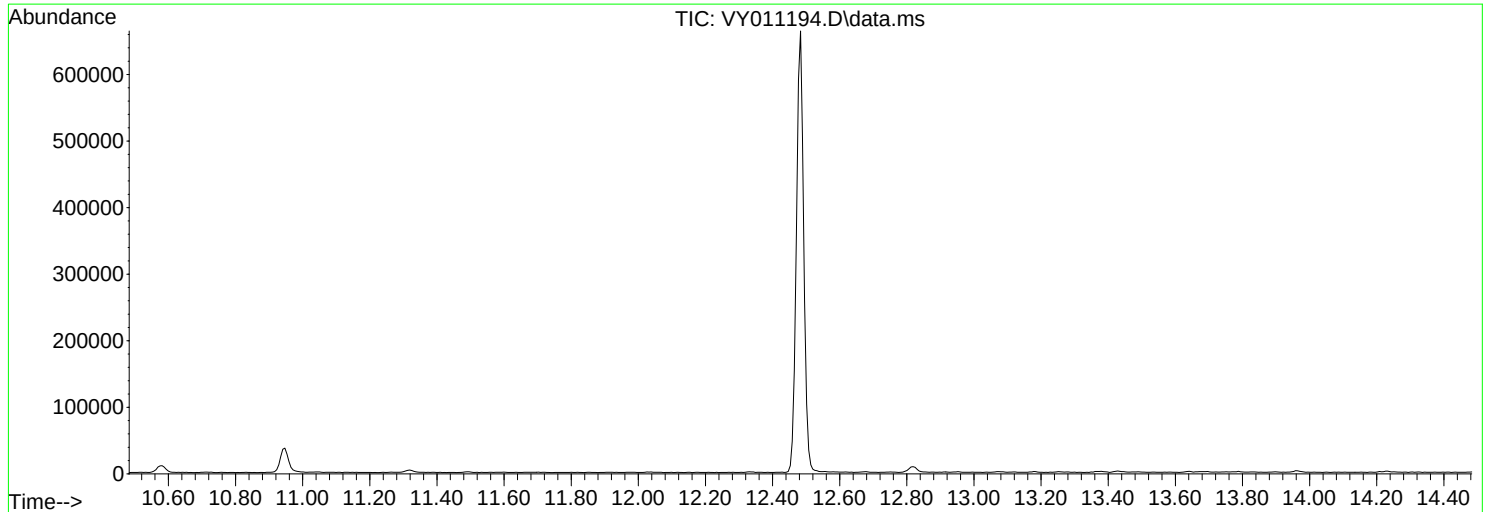

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	20621	PASS
75	95	30	60	49.8	59312	PASS
95	95	100	100	100.0	118981	PASS
96	95	5	9	6.7	8031	PASS
173	174	0.00	2	1.2	1175	PASS
174	95	50	100	80.7	95997	PASS
175	174	5	9	7.4	7126	PASS
176	174	95	101	95.5	91701	PASS
177	176	5	9	6.7	6100	PASS