


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY110119\
Data File : VY000516.D
Acq On : 01 Nov 2019 10:22
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

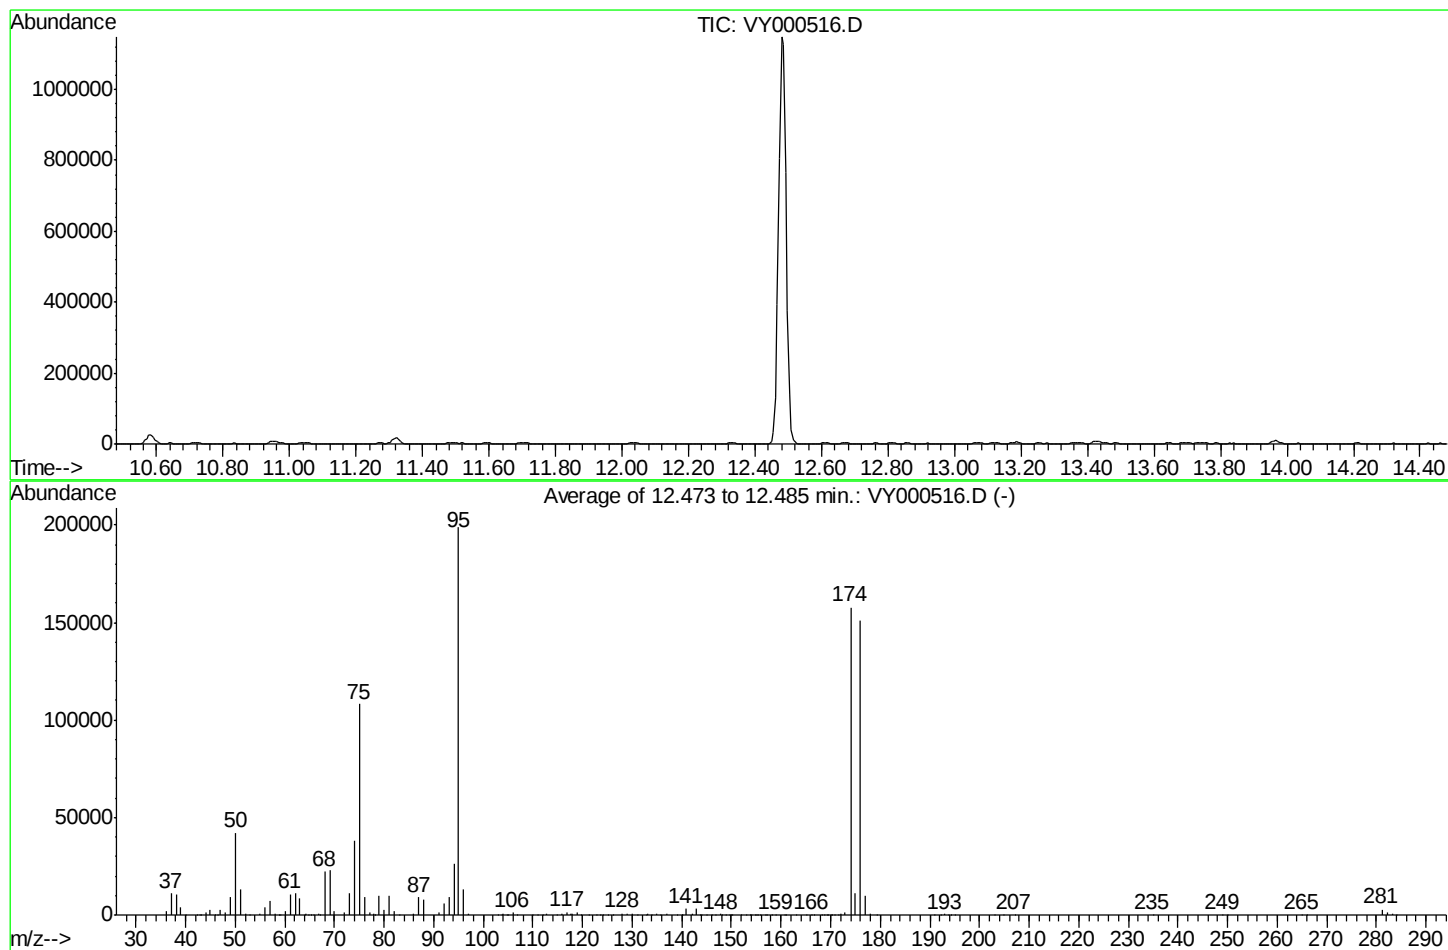

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	42330	PASS
75	95	30	60	54.4	108208	PASS
95	95	100	100	100.0	198826	PASS
96	95	5	9	6.6	13071	PASS
173	174	0.00	2	0.8	1204	PASS
174	95	50	100	79.3	157570	PASS
175	174	5	9	7.1	11220	PASS
176	174	95	101	95.9	151085	PASS
177	176	5	9	6.5	9811	PASS