
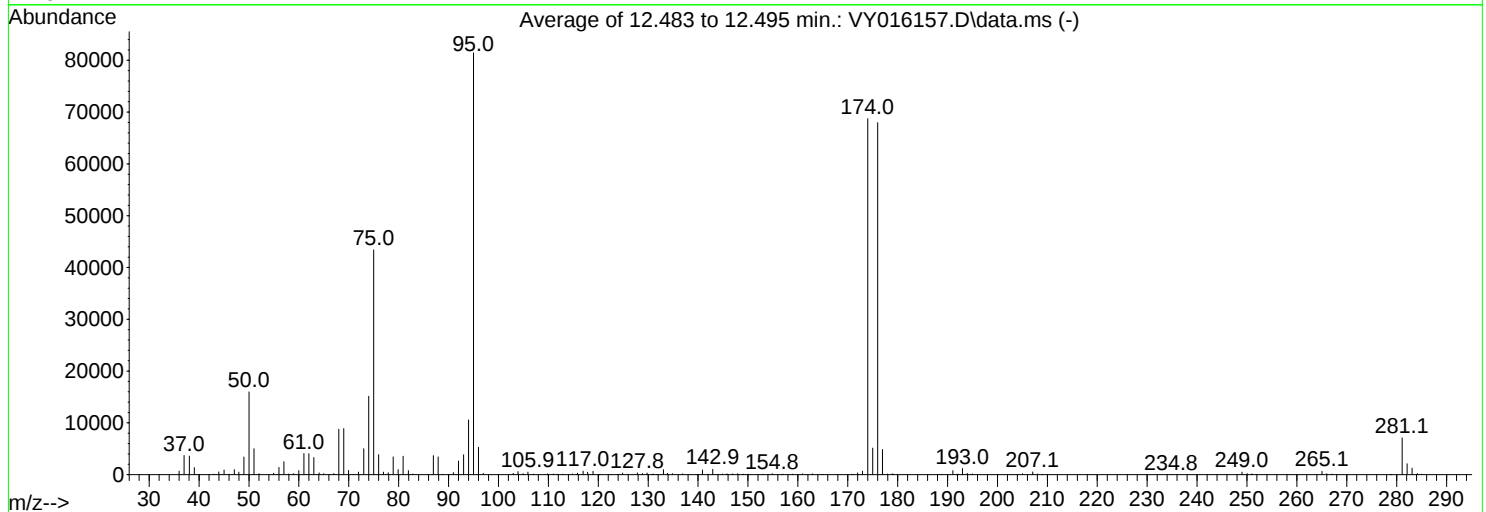


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110123\
Data File : VY016157.D
Acq On : 01 Nov 2023 08:48
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103123S.M
Title : SW846 8260
Last Update : Wed Nov 01 03:33:29 2023

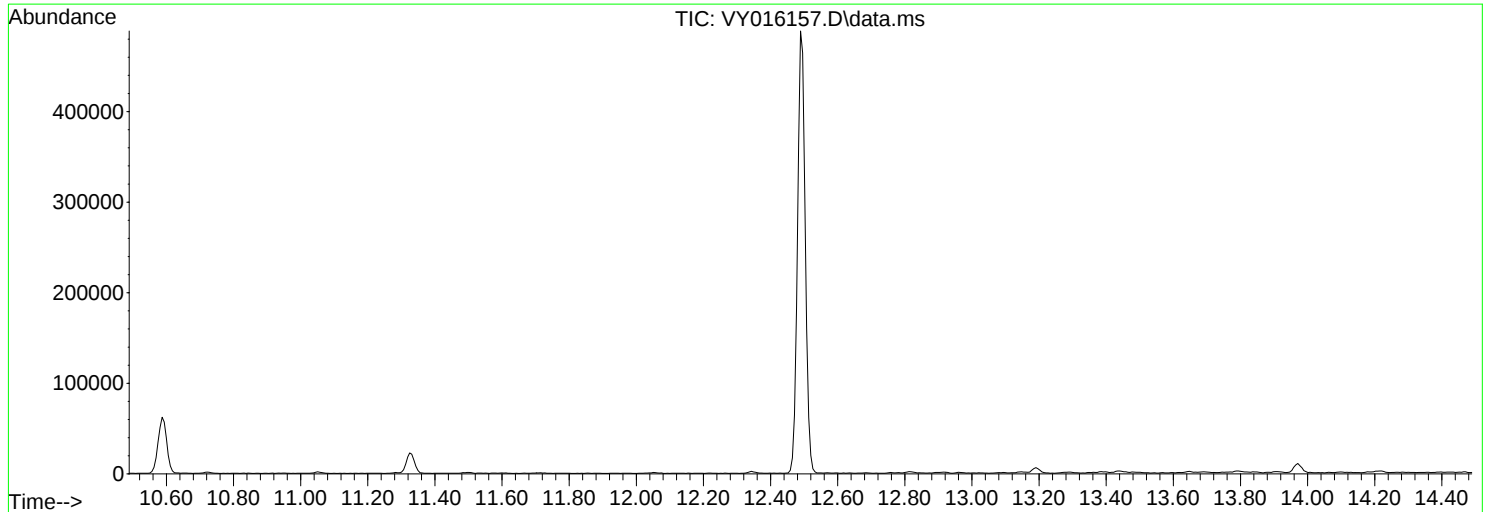

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	15985	PASS
75	95	30	60	53.3	43415	PASS
95	95	100	100	100.0	81443	PASS
96	95	5	9	6.5	5274	PASS
173	174	0.00	2	1.0	697	PASS
174	95	50	100	84.4	68752	PASS
175	174	5	9	7.5	5126	PASS
176	174	95	101	98.9	67981	PASS
177	176	5	9	7.2	4865	PASS