

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY110220\
 Data File : VY003474.D
 Acq On : 02 Nov 2020 15:49
 Operator : SY/MD
 Sample : L4565-02
 Misc : 5.70G/5ML/MSVOA Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FK-GF-02-063-A

Quant Time: Nov 03 02:25:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y110220S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 02 12:40:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	224654	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	354503	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	298522	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	126722	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	123951	53.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.64%	
35) Dibromofluoromethane	7.73	113	109751	50.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.76%	
50) Toluene-d8	10.18	98	417096	46.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.96%	
62) 4-Bromofluorobenzene	12.48	95	121835	40.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	81.94%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY110220\
Data File : VY003474.D
Acq On : 02 Nov 2020 15:49
Operator : SY/MD
Sample : L4565-02
Misc : 5.70G/5ML/MSVOA Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FK-GF-02-063-A

Quant Time: Nov 03 02:25:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y110220S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 02 12:40:51 2020
Response via : Initial Calibration

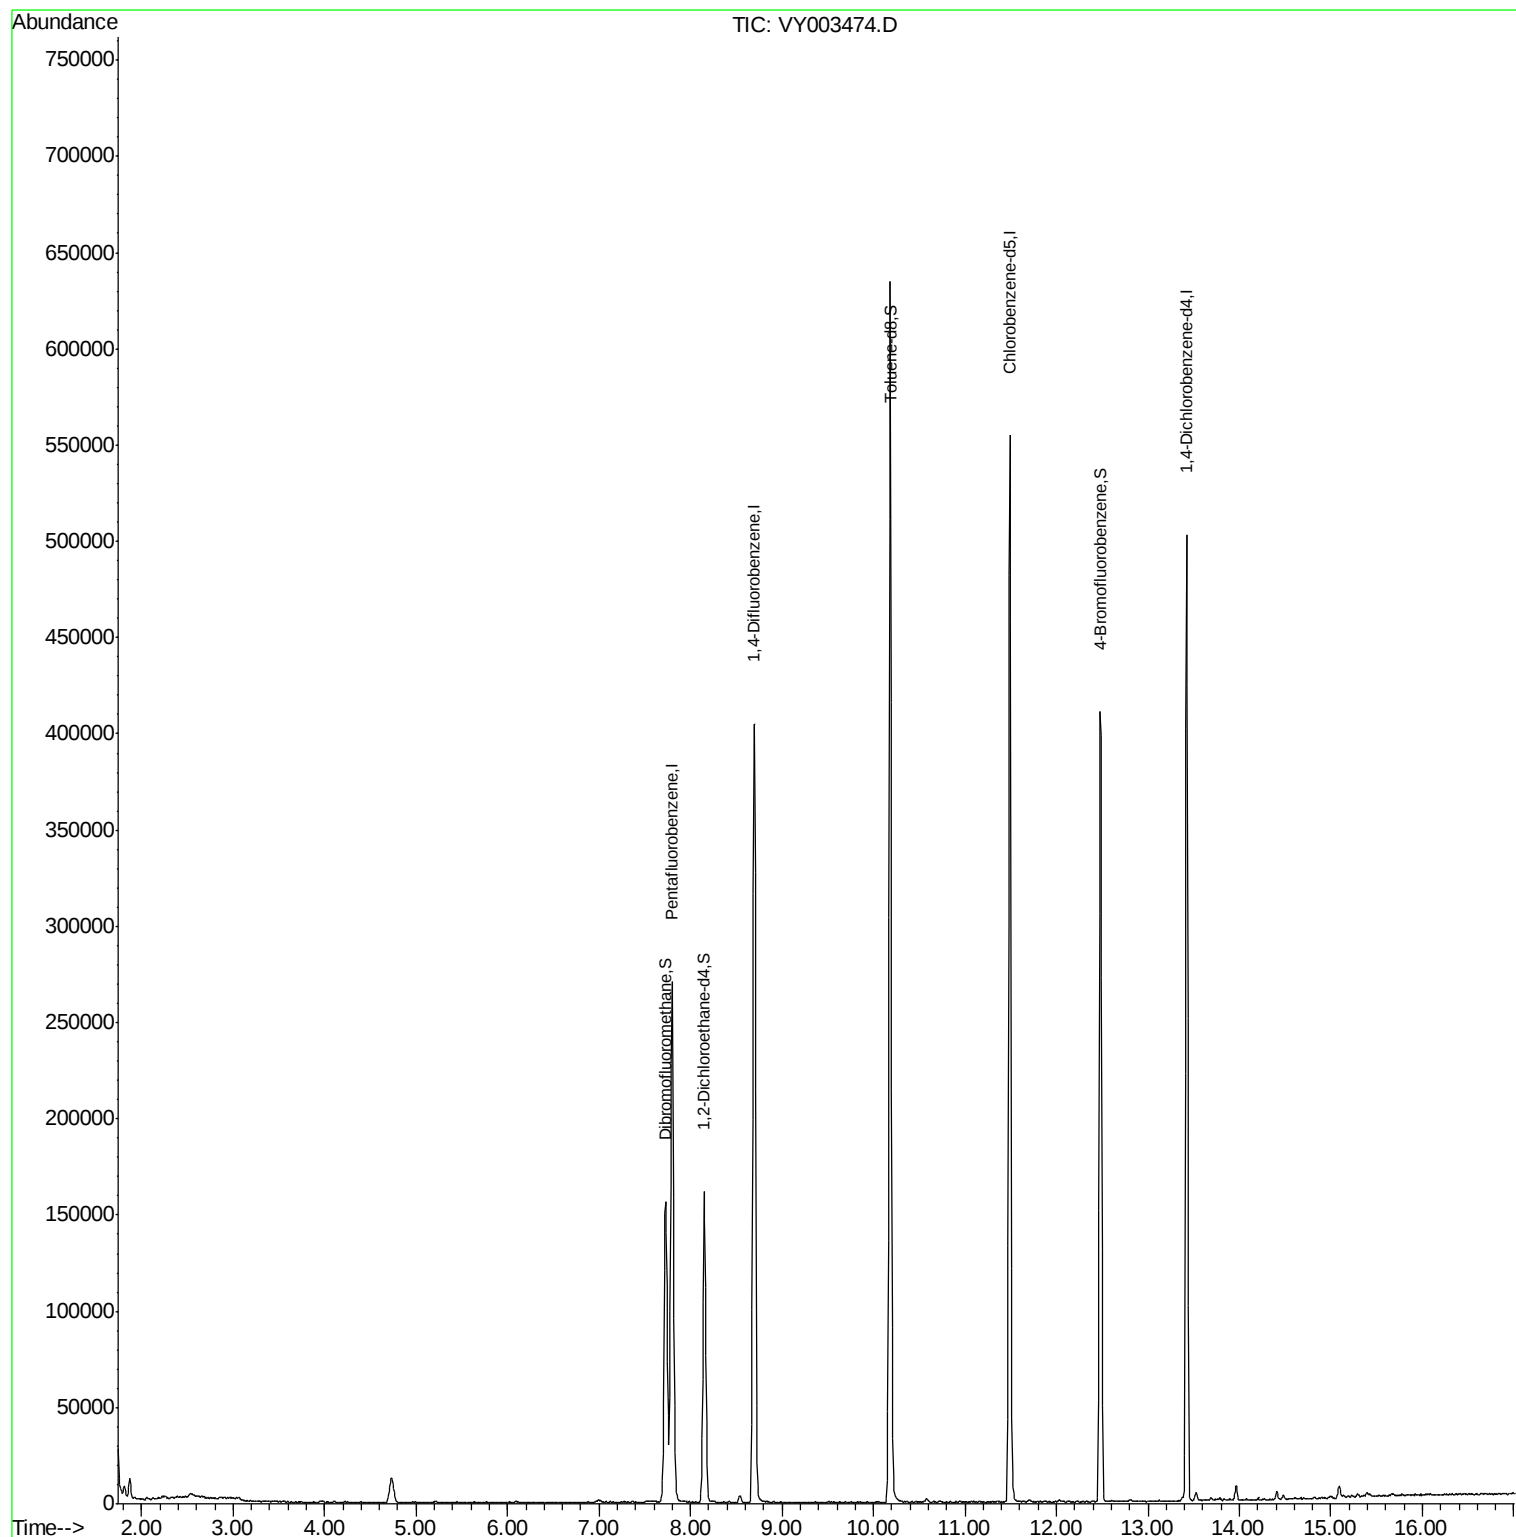



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.01 min

Lab File: VY003474.D

Acq: 02 Nov 2020 15:49

Instrument :

MSVOA_Y

ClientSampleId :


FK-GF-02-063-A

Tot Ion:168 Resp: 224654

Ion Ratio Lower Upper

168 100

99 50.7 39.7 59.5



Abundance Ion 167.90 (167.60 to 168.60): VY003464.D (-984) (-)

Ion 98.90 (98.60 to 99.60): VY003464.D (-984) (-)

7.80

100000

80000

60000



40000

20000

0

7.70 7.80 7.90

Time-->



#33

1,2-Dichloroethane-d4

Concen: 53.819 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY003474.D


Acq: 02 Nov 2020 15:49

Tgt Ion: 65 Resp: 123951

Ion Ratio Lower Upper

65 100

67 51.7 0.0 106.0



Abundance Ion 64.90 (64.60 to 65.60): VY003464.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY003464.D (-1041) (-)

8.15

60000


40000


20000

0

8.00 8.10 8.20 8.30

Time-->









#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.70 min Scan# 1142
 Delta R.T. -0.00 min
 Lab File: VY003474.D
 Acq: 02 Nov 2020 15:49




Instrument :
 MSVOA_Y
 ClientSampleId :
 FK-GF-02-063-A


Tot Ion:114 Resp: 354503
 Ion Ratio Lower Upper
 114 100
 63 20.2 0.0 40.6
 88 15.2 0.0 29.4

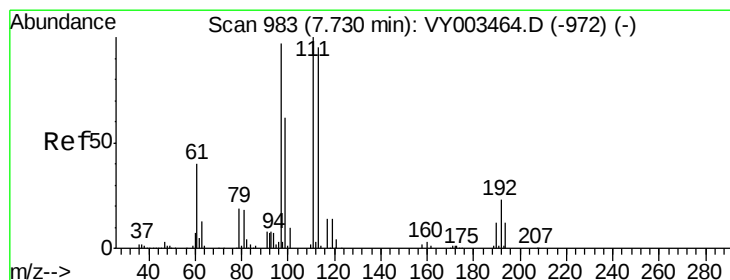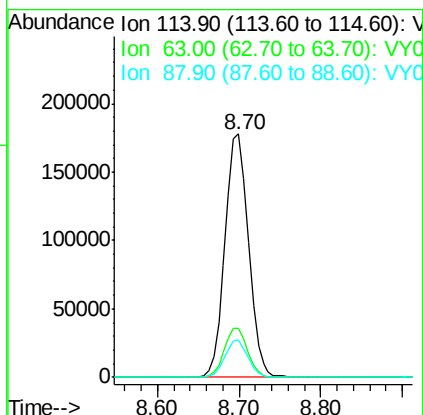

#35
 Dibromofluoromethane
 Concen: 50.876 ug/l
 RT: 7.73 min Scan# 983
 Delta R.T. -0.00 min
 Lab File: VY003474.D
 Acq: 02 Nov 2020 15:49

Tgt Ion:113 Resp: 109751
 Ion Ratio Lower Upper
 113 100
 111 102.5 81.8 122.6
 192 23.6 18.8 28.2

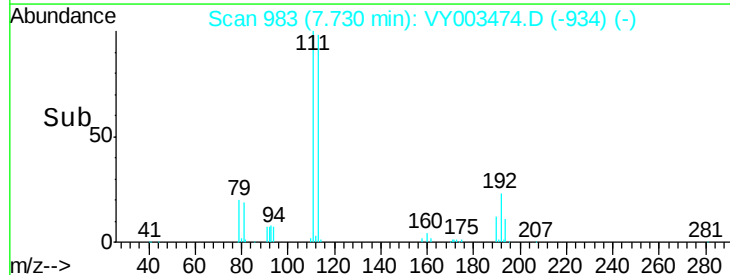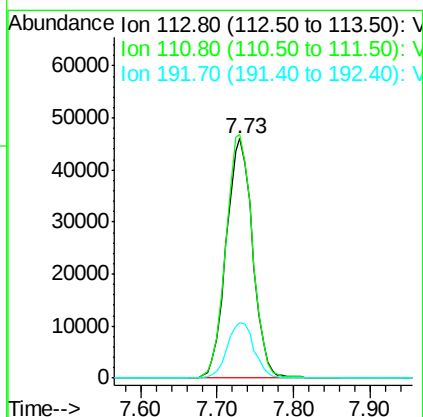



#50

Toluene-d8

Concen: 46.477 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY003474.D

Acq: 02 Nov 2020 15:49

Instrument :

MSVOA_Y

ClientSampleId :





FK-GF-02-063-A

Tot Ion: 98 Resp: 417096

Ion Ratio Lower Upper

98 100

100 64.0 50.9 76.3

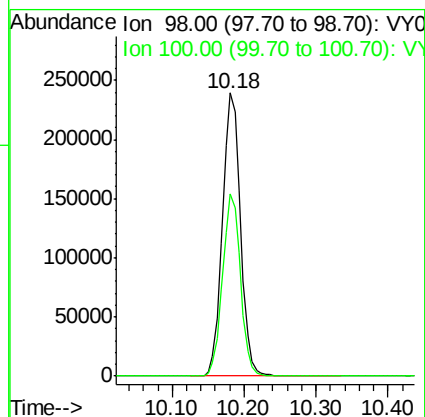

#62

4-Bromofluorobenzene

Concen: 40.974 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY003474.D

Acq: 02 Nov 2020 15:49




Tgt Ion: 95 Resp: 121835


Ion Ratio Lower Upper

95 100

174 95.7 0.0 193.0

176 92.0 0.0 187.4

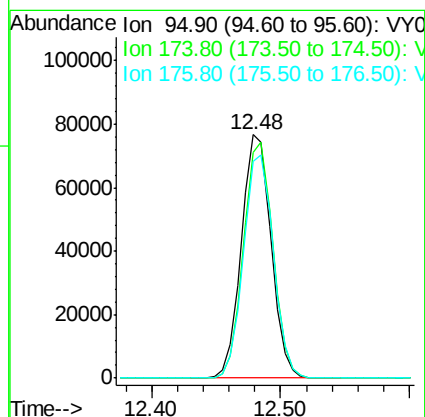







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.00 min
Lab File: VY003474.D
Acq: 02 Nov 2020 15:49

Instrument :
MSVOA_Y
ClientSampleId :
FK-GF-02-063-A

Tot Ion	Ratio	Lower	Upper
117	100		
82	54.9	43.4	65.2
119	32.8	25.8	38.6

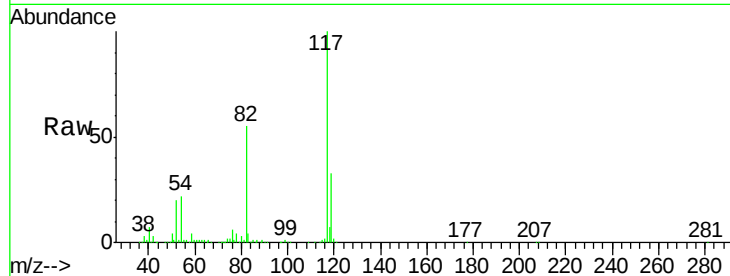


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

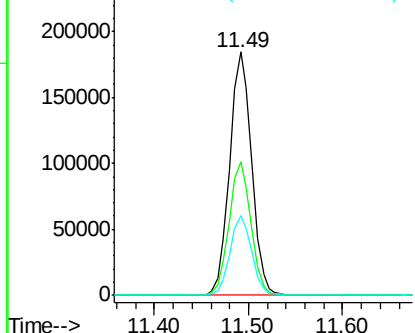

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY003474.D
Acq: 02 Nov 2020 15:49

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.4	27.5	82.4
150	157.5	0.0	345.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

