


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv110220\
 Data File : VY003460.D
 Acq On : 02 Nov 2020 09:14
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y110220S.M
 Title : SW846 8260
 Last Update : Mon Nov 02 12:40:51 2020

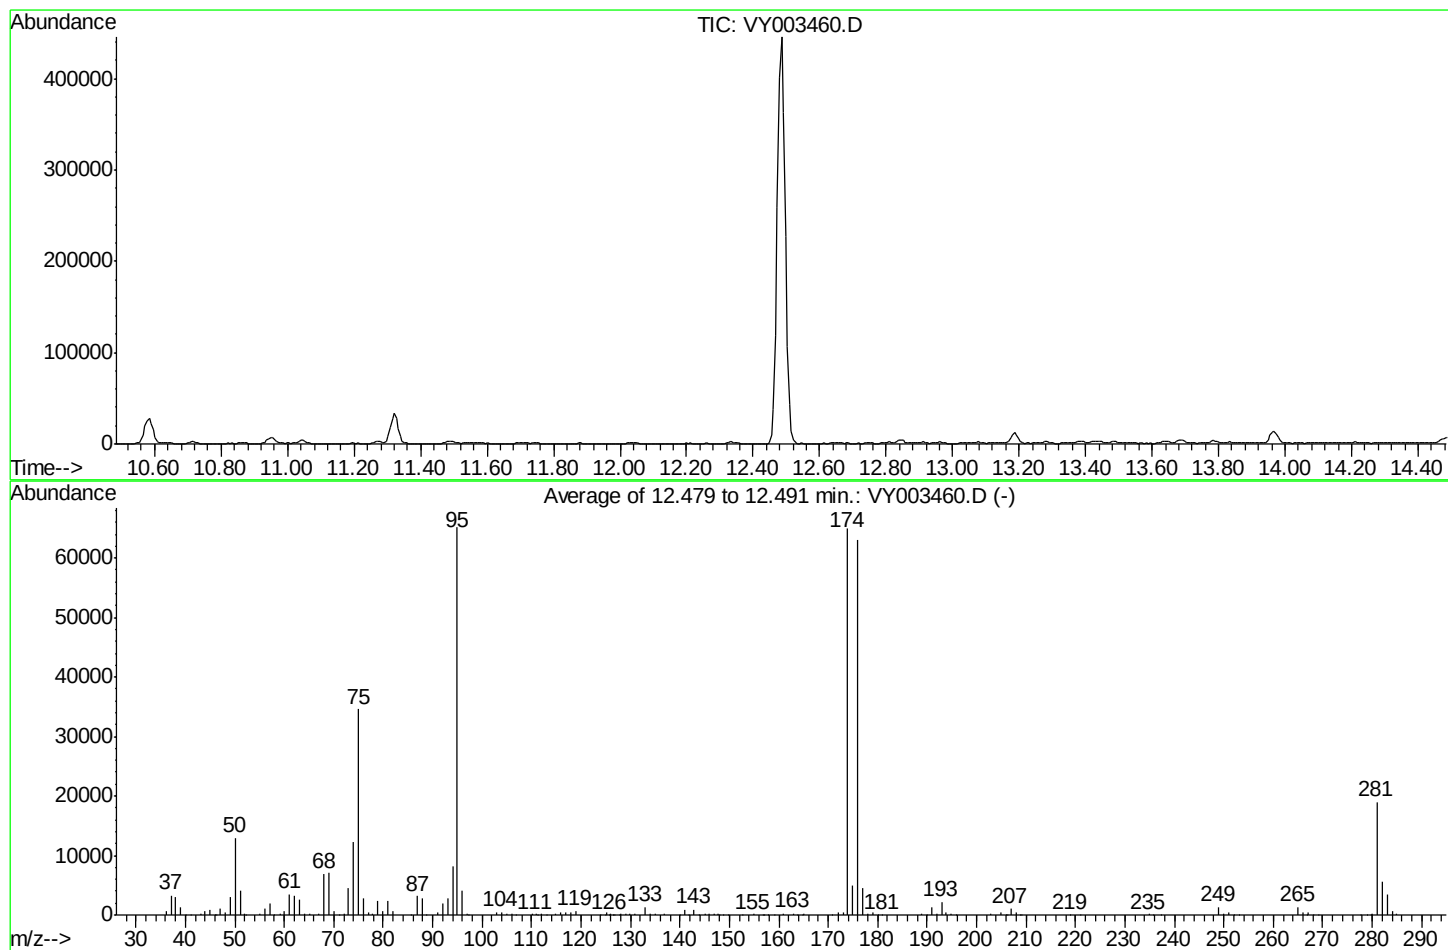

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	13024	PASS
75	95	30	60	53.1	34600	PASS
95	95	100	100	100.0	65170	PASS
96	95	5	9	6.3	4135	PASS
173	174	0.00	2	0.5	353	PASS
174	95	50	100	99.7	64946	PASS
175	174	5	9	7.5	4871	PASS
176	174	95	101	97.0	63008	PASS
177	176	5	9	7.3	4602	PASS