
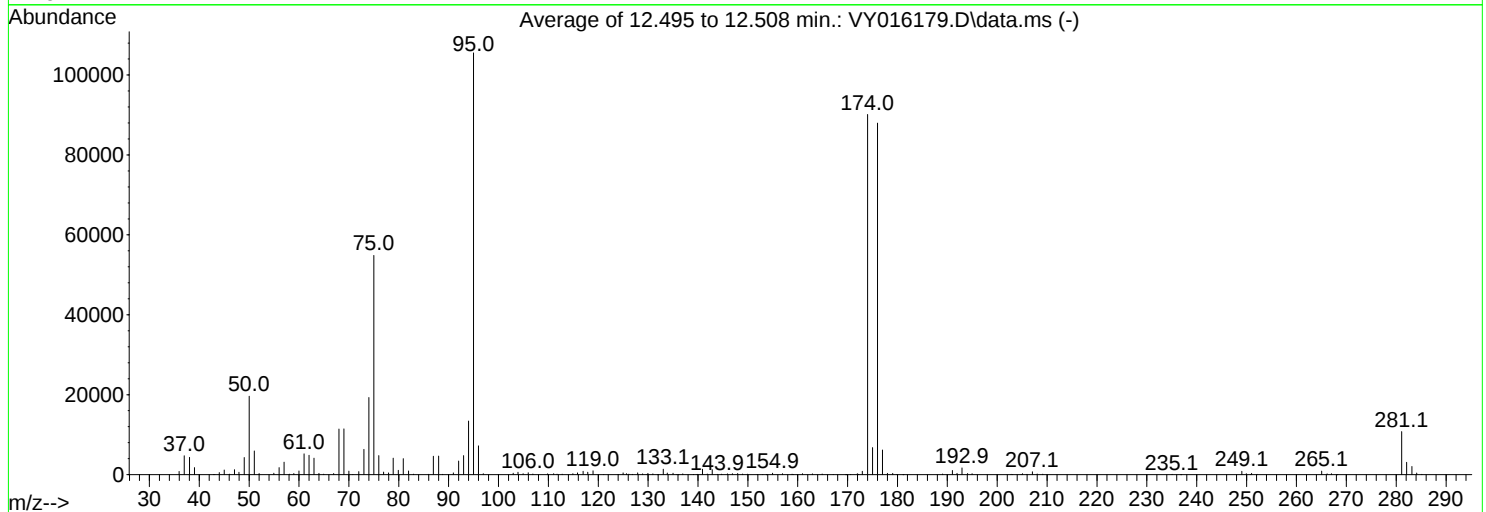


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110223\
Data File : VY016179.D
Acq On : 02 Nov 2023 08:31
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103123S.M
Title : SW846 8260
Last Update : Wed Nov 01 03:33:29 2023

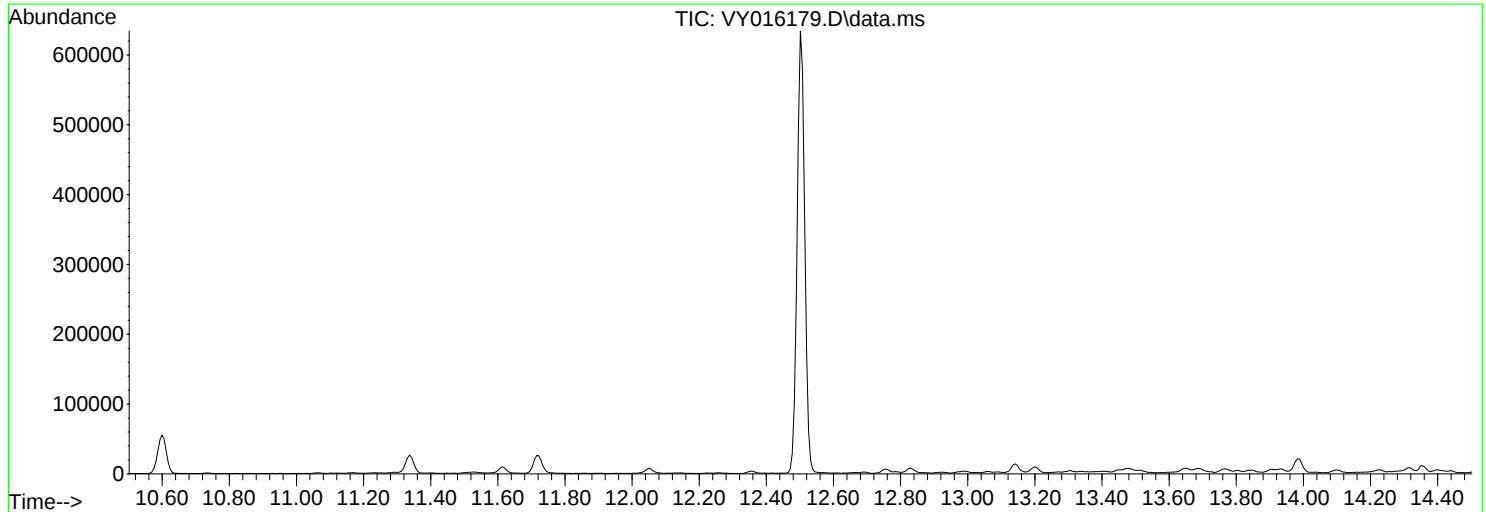

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	19608	PASS
75	95	30	60	52.0	54873	PASS
95	95	100	100	100.0	105549	PASS
96	95	5	9	6.8	7197	PASS
173	174	0.00	2	0.9	834	PASS
174	95	50	100	85.4	90147	PASS
175	174	5	9	7.5	6757	PASS
176	174	95	101	97.6	87971	PASS
177	176	5	9	7.0	6170	PASS