


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv110320\
Data File : VY003480.D
Acq On : 03 Nov 2020 09:17
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y110220S.M
Title : SW846 8260
Last Update : Mon Nov 02 12:40:51 2020

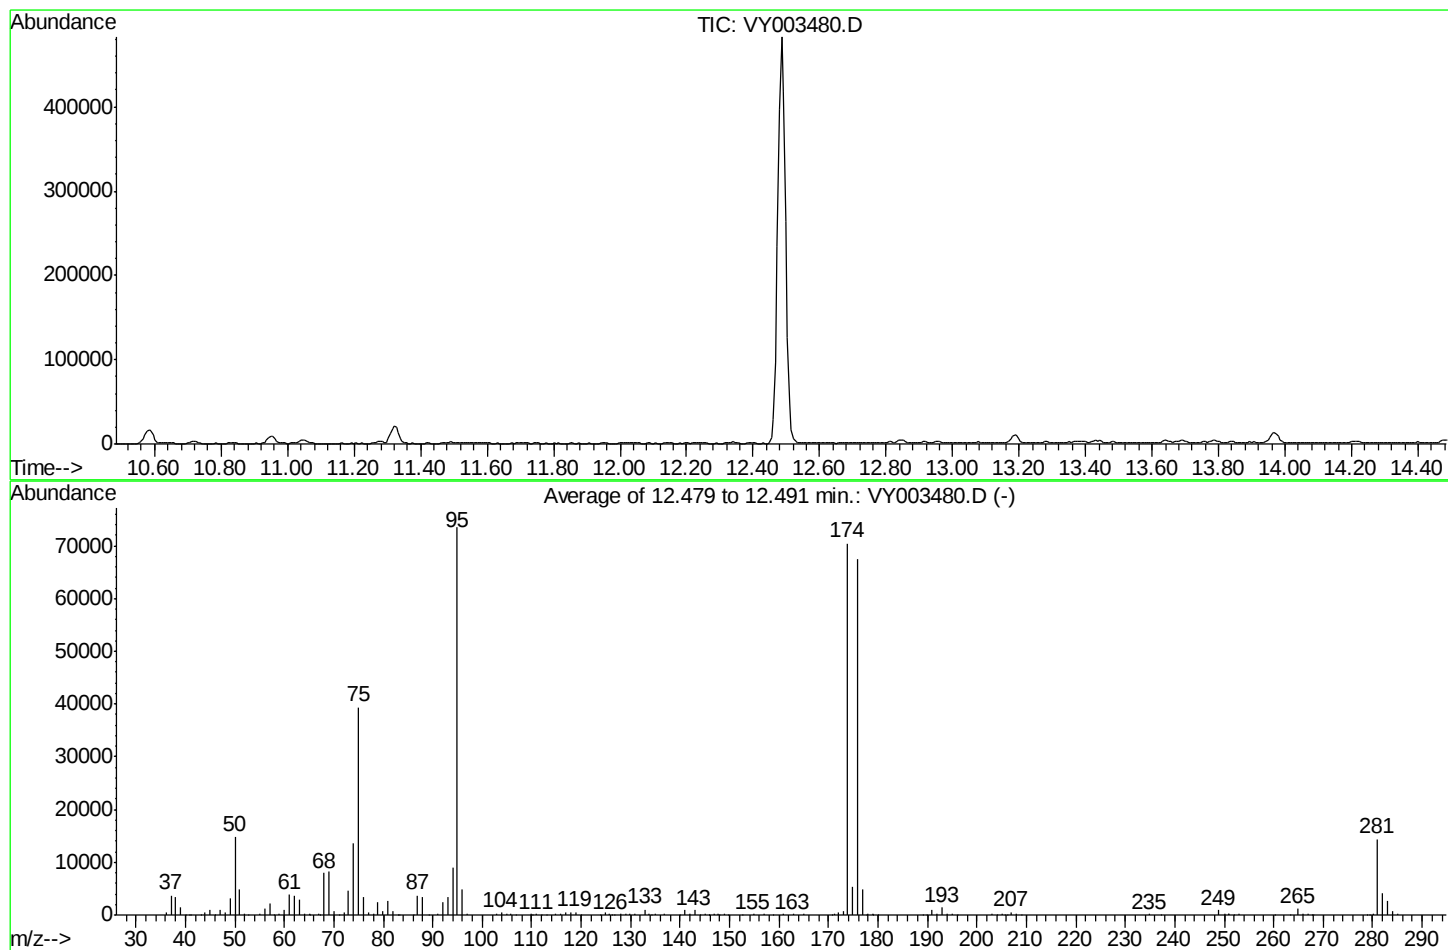

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	14821	PASS
75	95	30	60	53.6	39384	PASS
95	95	100	100	100.0	73501	PASS
96	95	5	9	6.7	4927	PASS
173	174	0.00	2	1.0	716	PASS
174	95	50	100	95.9	70469	PASS
175	174	5	9	7.7	5427	PASS
176	174	95	101	95.8	67520	PASS
177	176	5	9	7.0	4750	PASS